

# Spectrophotometric Measurement of Carbonate Ion in Seawater over a Decade: Dealing with Inconsistencies

Elisa F. Guallart,<sup>\*,□</sup> Noelia M. Fajar, Maribel I. García-Ibáñez, Mónica Castaño-Carrera, Rocío Santiago-Doménech, Abed El Rahman Hassoun, Fiz F. Pérez, Regina A. Easley, and Marta Álvarez<sup>□</sup>



Cite This: *Environ. Sci. Technol.* 2022, 56, 7381–7395



Read Online

ACCESS |



Metrics & More




Article Recommendations



Supporting Information

**ABSTRACT:** The spectrophotometric methodology for carbonate ion determination in seawater was first published in 2008 and has been continuously evolving in terms of reagents and formulations. Although being fast, relatively simple, affordable, and potentially easy to implement in different platforms and facilities for discrete and autonomous observations, its use is not widespread in the ocean acidification community. This study uses a merged overdetermined  $\text{CO}_2$  system data set (carbonate ion, pH, and alkalinity) obtained from 2009 to 2020 to assess the differences among the five current approaches of the methodology through an internal consistency analysis and discussing the sources of uncertainty. Overall, the results show that none of the approaches meet the climate goal ( $\pm 1\%$  standard uncertainty) for ocean acidification studies for the whole carbonate ion content range in this study but usually fulfill the weather goal ( $\pm 10\%$  standard uncertainty). The inconsistencies observed among approaches compromise the consistency of data sets among regions and through time, highlighting the need for a validated standard operating procedure for spectrophotometric carbonate ion measurements as already available for the other measurable  $\text{CO}_2$  variables.

**KEYWORDS:** ocean acidification, saturation states, bio-geochemistry, oceanic carbon cycle, time-series,  $\text{CO}_2$  system monitoring,  $\text{CO}_2$  system variables, climate goal

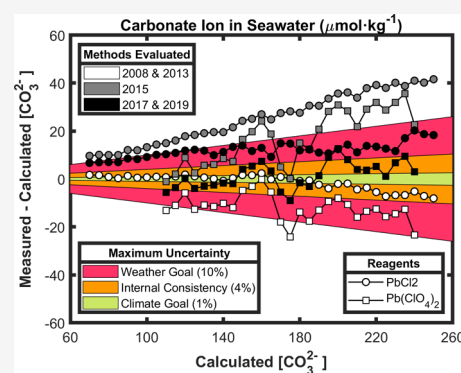

## 1. INTRODUCTION

About a third of the global anthropogenic carbon dioxide ( $\text{CO}_2$ ) emissions have been absorbed by the global ocean since the preindustrial era.<sup>1</sup> By acting as a sink of atmospheric  $\text{CO}_2$ , the ocean contributes to decreasing the rate at which climate change occurs. Nevertheless, such an effect is counteracted by the resulting increase in seawater acidity (ocean acidification, OA), which determines a decrease in the amount of carbonate ion content in seawater ( $[\text{CO}_3^{2-}]$ ) and therefore of buffering capacity of the ocean.<sup>2–6</sup>

The overall concern for the sustainability of marine life and resources has mobilized the international community to coordinate efforts to track long-term trends in OA by observing seawater  $\text{CO}_2$  variables in coastal<sup>7</sup> and open ocean<sup>8,9</sup> time-series. The measurable seawater  $\text{CO}_2$  variables (dissolved inorganic carbon (DIC), total alkalinity (TA), partial pressure of  $\text{CO}_2$  ( $p\text{CO}_2$ ), and pH) are included by the Global Ocean Observing System (GOOS) as Essential Ocean Variables (EOVs) to constrain the  $\text{CO}_2$  system changes and drivers in seawater. Identified and predicted bio-geochemical<sup>10,11</sup> and ecological<sup>12–14</sup> OA implications are related to changes in the saturation state ( $\Omega$ ) of seawater for calcium carbonate ( $\text{CaCO}_3$ ) minerals,<sup>2,11,15</sup> which control the precipitation and dissolution of its aragonite and calcite forms depending on the available in

situ  $[\text{CO}_3^{2-}]$ .<sup>16</sup> As the oceans acidify, the location and extent of the regions where  $\text{CaCO}_3$  dissolution occurs are expected to increase,<sup>11,15</sup> particularly in regions with low buffer capacity (Appendix A in Supporting Information).

The increasing amount of  $\text{CO}_2$  data produced demands quality-controlled measurements to ensure their intercomparison. Regarding the four measurable seawater  $\text{CO}_2$  system variables, standard procedures of analysis, data quality control, and reporting are widely established.<sup>17,18</sup> Additionally, to improve the spatiotemporal resolution of the observation of the seawater  $\text{CO}_2$  system, intensive effort has been made to implement standardized procedures for in situ autonomous measurements performed by autonomous vehicles.<sup>19,20</sup> Accordingly, relatively simple, fast, and precise automated methods for discrete measurements are encouraged to be implemented.<sup>21</sup> In this regard, most studies would benefit from moving  $[\text{CO}_3^{2-}]$

**Received:** September 8, 2021

**Revised:** April 12, 2022

**Accepted:** April 13, 2022

**Published:** June 7, 2022



from its category of a derived variable to become the fifth measurable seawater CO<sub>2</sub> system variable, thus allowing efficient ways of approaching questions relative to CaCO<sub>3</sub> cycling from [CO<sub>3</sub><sup>2-</sup>] direct determinations.<sup>22,23</sup> To this end, Byrne and Yao<sup>24</sup> first proposed a spectrophotometric method to determine [CO<sub>3</sub><sup>2-</sup>] in seawater. This method is proposed to be ready for implementation in sustained observations and internal consistency studies.<sup>25,26</sup> However, its implementation still needs to be validated by independent research groups.

The methodology for the quantification of spectrophotometric [CO<sub>3</sub><sup>2-</sup>] ([CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub>) relies on the speciation of lead (Pb(II)) in seawater over a particular pH range (7.7–8.2) at which the complexation of Pb(II) and CO<sub>3</sub><sup>2-</sup> predominantly occurs.<sup>27</sup> The main details on the theory behind the methodology and its evolution are summarized below. A detailed explanation of the motivation for such methodological changes can be found in the [Supporting Information](#) (Appendix B) and the related literature.<sup>24,25,27–33</sup>

[CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub> is determined by quantifying the ultraviolet light absorbed by lead carbonate, lead chloride/sulfate species, and free Pb<sup>2+</sup> in Pb(II)-enriched seawater through the following expression:

$$-\log[\text{CO}_3^{2-}]_{\text{spec}} = \log\left[\frac{\text{CO}_3\beta_1}{e_2}\right] + \log\left[\frac{R - e_1}{1 - R \cdot \frac{e_3}{e_2}}\right] \quad (1)$$

where CO<sub>3</sub>β<sub>1</sub> is the associated equilibrium constant for the complexation of Pb<sup>2+</sup> and [CO<sub>3</sub><sup>2-</sup>], and *R* is the absorbance (*A*) ratio of Pb(II) species at 234 nanometers (nm) and 250 nm, corrected for the background absorbance at 350 nm:

$$R = \frac{250A - 350A}{234A - 350A} \quad (2)$$

The molar absorptivity ratios *e*<sub>1</sub>, *e*<sub>2</sub>, and *e*<sub>3</sub>/*e*<sub>2</sub> are defined as

$$e_1 = \frac{250 \epsilon_{\text{PbCO}_3}}{234 \epsilon_{\text{PbCO}_3}}, \quad e_2 = \frac{250 \epsilon_{\text{Pb}}}{234 \epsilon_{\text{PbCO}_3}}, \quad e_3/e_2 = \frac{234 \epsilon_{\text{Pb}}}{250 \epsilon_{\text{Pb}}} \quad (3)$$

**Equation 1** has the same form as the one used to determine spectrophotometric pH on the total pH scale<sup>34</sup> and allows quantifying [CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub> with a minimum number of parameters via a procedure that closely follows that of spectrophotometric pH. However, unlike other measurable CO<sub>2</sub> system variables, no recommended standard operating procedure (SOP) has been established for measuring [CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub>, nor are certified reference materials (CRMs) available for this variable.<sup>17</sup>

The first approach for measuring [CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub> was described by Byrne and Yao<sup>24</sup> in 2008 (BY08). During the following decade, the method was refined by Easley et al.<sup>28</sup> (EAS13), Patsavas et al.<sup>29</sup> (PAT15), Sharp et al.<sup>30</sup> (SHA17), and Sharp and Byrne<sup>25</sup> (SHA19) in terms of the procedure for obtaining accurate *R* data and, more importantly, the calibration or fitting of the parameters log{CO<sub>3</sub>β<sub>1</sub>/*e*<sub>2</sub>}, *e*<sub>1</sub>, and *e*<sub>3</sub>/*e*<sub>2</sub> (**eq 1**) needed to relate a particular *R* value (**eq 2**) with [CO<sub>3</sub><sup>2-</sup>] (**Appendix B**).

The former works of BY08 and EAS13 used Pb(II) chloride (PbCl<sub>2</sub>) as the reagent to obtain the *R* measurements. PAT15 proposed a change to Pb(II) perchlorate (Pb(ClO<sub>4</sub>)<sub>2</sub>) and recommended an additional procedure to correct *R* data for sample perturbation due to reagent addition, as

$$\log(R - R^0) = -17.6664 \cdot R^2 + 19.8995 \cdot R - 7.7324 \quad (4)$$

where *R*<sup>0</sup> corresponds to the unperturbed *R* value. After SHA17, *R* measurements were no longer corrected with **eq 4** but readjusted to include an offset correction for wavelength calibration inaccuracies of the spectrophotometer (*R*<sup>0</sup>), as


$$R^0 = R + 0.0265 \cdot \Delta\lambda_{241.1} \quad (5)$$

where Δλ<sub>241.1</sub> is the spectrophotometer-specific wavelength offset, defined as the difference between the wavelength location of a holmium oxide standard absorbance peak at 241.10 nm specified by the manufacturer minus the wavelength at which the spectrophotometer reports the peak. The sign of **eq 5** is reversed with regard to SHA17, where there was an error in the reported equation (J. D. Sharp, personal communication). *R*<sup>0</sup> refers to the true *R* value for PAT15 and SHA17. Finally, SHA19 followed SHA17 to obtain *R*<sup>0</sup> but reported the most recent characterization of the terms in **eq 1**, extending their suitability to a larger range of temperatures and salinities. Before SHA19, the method was solely characterized for use at 25 °C.

All five approaches (**Table S1**) for [CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub> determination are valid for given oceanographic conditions, and none clearly invalidates the others.<sup>24,25,28–30</sup> In this study, the evolution of the [CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub> methodology is evaluated through an internal consistency analysis of a field-based data set obtained during 2009–2020 and expanding over a broad range of oceanographic conditions. A detailed assessment of the different sources of uncertainty in [CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub> is discussed. Finally, difficulties found concerning the implementation of the methodology are highlighted.

## 2. MATERIALS AND METHODS

**2.1. Cruise Data Compilation.** Hydrographic and chemical data from nine open ocean cruises in the North Atlantic Ocean and the Mediterranean Sea, and one coastal time-series in the North-East Atlantic Ocean, performed during 2009–2020 (**Figure 1** and **Table 1**), were compiled for assessing the evolution of the [CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub> methodology. All data sets include paired measurements of [CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub>, pH, and TA, and some also include DIC measurements. All seawater CO<sub>2</sub> system variables were measured following the corresponding SOPs<sup>17</sup> except

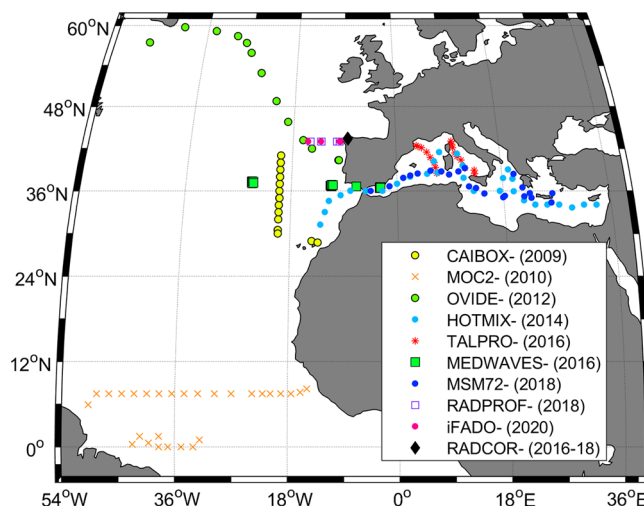

**Figure 1.** Location of the hydrographic stations of nine open ocean cruises and one coastal time-series site where spectrophotometric carbonate ion content ([CO<sub>3</sub><sup>2-</sup>]<sub>spec</sub>), pH, TA, and DIC were measured, during 2009–2020. See **Table 1** for further details.

Table 1. Cruise Summary Information Containing the Cruise Alias and Assigned EXPCODE, Research Vessel and Year of Performance, and Ocean Region Studied<sup>a</sup>

Cruise Alias, EXPCODE	Research vessel, year	Region	Pb(II) reagent(N)	Precision mean $\pm$ STD ( $\mu\text{mol}\cdot\text{kg}^{-1}$ ) (%)	spectroph. $[\text{CO}_3^{2-}]_{\text{spec}}/\text{pH}$	Salinity range	pH range	TA range ( $\mu\text{mol}\cdot\text{kg}^{-1}$ )	$[\text{CO}_3^{2-}]_{\text{calc}}\text{range}$ ( $\mu\text{mol}\cdot\text{kg}^{-1}$ )	TA/DIC range
CAIBOX, 29AH20090725	R/V Sarmiento de Gamboa, 2009	North East Atlantic	PbCl <sub>2</sub> (272)	225.0 $\pm$ 2.9 (1.3 %)	PE850/SHI2401	34.89–37.08	7.65–8.03	2305–2428	101–227	1.05–1.15
MOC2, 29HE20100405	R/V Hesperides, 2010	Equatorial Atlantic	PbCl <sub>2</sub> (625)	249.0 $\pm$ 3.4 (1.4 %)	SHI2401	34.50–36.72	7.47–8.13	2294–2408	68–252	1.02–1.18
HOTMIX, 29AH20140426	R/V Meteor, 2011	Mediterranean Sea	PbCl <sub>2</sub> (328)	214.0 $\pm$ 2.6 (1.2 %)	SHI2600	34.89–39.24	7.72–8.02	2330–2634	118–250	1.07–1.15
OVIDE, 29AH20120623	R/V Sarmiento de Gamboa, 2012	Subpolar North Atlantic	PbCl <sub>2</sub> (196)	129.0 $\pm$ 1.6 (1.2 %)	PE850	34.46–36.23	7.69–7.99	2292–2398	109–201	1.06–1.13
TALPRO, 29AJ20160818	R/V Angeles Alvarino, 2016	Western Mediterranean Sea	Pb(ClO <sub>4</sub> ) <sub>2</sub> (115)	211.0 $\pm$ 7.0 (4 %)	BK800	37.30–38.82	7.88–8.02	2476–2620	187–242	1.11–1.15
MEDWAVES, N/A	R/V Sarmiento de Gamboa, 2016	North Eastern Atlantic and Alboran Sea	Pb(ClO <sub>4</sub> ) <sub>2</sub> (148)	131.0 $\pm$ 1.0 (0.6 %)	PE850	34.93–38.54	7.70–8.01	2310–2590	111–212	1.06–1.14
MSM72, 06M22010302	R/V Maria S. Merian, 2018	Mediterranean Sea	Pb(ClO <sub>4</sub> ) <sub>2</sub> (294)	238.0 $\pm$ 1.0 (0.4 %)	SHI2600	36.45–39.29	7.86–7.99	2397–2639	179–239	1.10–1.14
RADPROF, N/A	R/V Ramon Margalef, 2018	Iberian Basin North East Atlantic	PbCl <sub>2</sub> (50)	131.0 $\pm$ 0.8 (0.6 %)	SHI2600	34.90–36.02	7.72–7.97	2316–2383	116–193	1.07–1.13
RADCOR, N/A	R/V-Lura, 2016 to 2018	North West Galician Coast	Pb(ClO <sub>4</sub> ) <sub>2</sub> (46)	126.0 $\pm$ 2.5 (2 %)	SHI2600	33.72–35.74	7.78–8.02	2249–2361	131–200	1.08–1.14
iFADO, N/A	R/V Sarmiento de Gamboa, 2020	Iberian Basin North East Atlantic	Pb(ClO <sub>4</sub> ) <sub>2</sub> (74)	126.0 $\pm$ 2.2 (1.7 %)	SHI2600	34.89–36.13	7.72–7.96	2315–2390	115–188	1.07–1.13
iFADO2, N/A	R/V Sarmiento de Gamboa, 2020	Iberian Basin North East Atlantic	Pb(ClO <sub>4</sub> ) <sub>2</sub> (32)	122.0 $\pm$ 1.0 (1 %)	PE850/SHI2600	34.89–36.13	7.72–7.96	2315–2389	115–188	1.07–1.13
			Pb(ClO <sub>4</sub> ) <sub>2</sub> (34)	122.0 $\pm$ 2.0 (1.7 %)						

<sup>a</sup>Information relative to  $[\text{CO}_3^{2-}]_{\text{spec}}$ : Pb(II) reagent and number of measurements (N); precision in  $\mu\text{mol}\cdot\text{kg}^{-1}$  and % (mean  $[\text{CO}_3^{2-}]_{\text{spec}} \pm$  standard deviation, STD, of the measured replicates is also shown). The spectrophotometer (spectroph.) used for obtaining  $[\text{CO}_3^{2-}]_{\text{spec}}$  and pH is indicated. The ranges of main variables are shown: salinity, pH (total scale at 25 °C), total alkalinity (TA), calculated carbonate ion content ( $[\text{CO}_3^{2-}]_{\text{calc}}$  at 25 °C from pH-TA pair), and TA/DIC ratio (DIC calculated from pH-TA). The reagent PbCl<sub>2</sub> was 1.1 mmol·L<sup>-1</sup>, and 250  $\mu\text{L}$  (CAIBOX, MOC2, and OVIDE) or 225  $\mu\text{L}$  (rest of cruises) were added. The Pb(ClO<sub>4</sub>)<sub>2</sub> reagent was 22 mmol·L<sup>-1</sup>, and 20  $\mu\text{L}$  were added.



$[\text{CO}_3^{2-}]_{\text{spec}}$  that lacks an SOP. As ancillary data, this study uses hydrographic CTD data and inorganic nutrients (silicate and phosphate). The compiled data set is publicly available in Alvarez et al.<sup>35</sup>

A solution of unpurified *m*-cresol purple ( $2 \text{ mmol}\cdot\text{L}^{-1}$ ) was used for spectrophotometric pH measurements.<sup>34</sup> All pH data are reported on the total hydrogen ion scale at  $25^\circ\text{C}$  and atmospheric pressure (hereafter pH). The overall pH precision for all cruises is  $\pm 0.003$  pH units based on sample replicates, while the assigned total uncertainty is considered as  $\pm 0.01$  pH units (Appendix C).<sup>36–38</sup> TA samples were measured following a double end-point potentiometric titration,<sup>39–41</sup> and DIC samples were analyzed through coulometric determination.<sup>42</sup> TA and DIC accuracies were verified with CRMs.<sup>43</sup> The TA and DIC precision is  $\pm 2 \mu\text{mol}\cdot\text{kg}^{-1}$  based on sample replicates, and the total uncertainty is  $\pm 3 \mu\text{mol}\cdot\text{kg}^{-1}$  for both TA and DIC.<sup>36</sup> pH and TA measurements were performed onboard except for the RADCOR time-series, where samples were analyzed at the Instituto Español de Oceanografía (IEO) laboratory the same day and within 2 days after sampling, respectively. DIC measurements were mostly performed postcruise at the IEO laboratory on stored samples poisoned with a saturated solution of mercuric chloride ( $\text{HgCl}_2$ ), except for the TALPRO and MSM72 cruises during which DIC measurements were performed onboard. Further cruise details are in Table 1.

The overall  $[\text{CO}_3^{2-}]_{\text{spec}}$  measurement procedure has remained the same during the study period. Seawater samples were collected from the Niskin bottles directly into 10 cm quartz cuvettes ( $\sim 30 \text{ mL}$  volume) that were immediately capped with Teflon caps and heated to  $25^\circ\text{C}$ . All spectrophotometric analyses were performed manually. For each cuvette, a baseline (seawater only) measurement was first performed and followed by the addition of the Pb(II) reagent. Absorbance measurements were recorded in triplicate at three wavelengths (234 nm, 250 nm, and 350 nm) to get an averaged absorbance ratio ( $R$ ; eq 2) for each sample. The temperature of each sample was recorded immediately with a temperature probe ( $\pm 0.03^\circ\text{C}$ ) after the absorbance measurements. The Pb(II) reagent, stock concentration, volume addition, and spectrophotometer used for each cruise are detailed in Table 1. Spectrophotometer specifications are detailed in Table S3. Except for CAIBOX and iFADO, pH and  $[\text{CO}_3^{2-}]_{\text{spec}}$  samples were always analyzed with the same spectrophotometer (Table 1). For iFADO, two different spectrophotometers were used onboard for comparison. The precision of the  $[\text{CO}_3^{2-}]_{\text{spec}}$  measurements was evaluated through replicate analysis during each cruise and ranged between  $\pm 1 \mu\text{mol}\cdot\text{kg}^{-1}$  and  $\pm 6.9 \mu\text{mol}\cdot\text{kg}^{-1}$  ( $\pm 0.4\%$  and  $\pm 4\%$ ) (Table 1).

One of the main analytical changes in the methodology reported during the study period implies a change in the Pb(II) reagent from  $\text{PbCl}_2$  (BY08 and EAS13) to  $\text{Pb}(\text{ClO}_4)_2$  (PAT15, SHA17, and SHA19) (Appendix B). In this study, 1666 samples were measured with  $\text{PbCl}_2$  in cruises performed during 2009–2012 (CAIBOX, MOC2, HOTMIX, and OVIDE), and 743 with  $\text{Pb}(\text{ClO}_4)_2$  during 2016–2020 (TALPRO, MEDWAVES, and MSM72). Double measurements with  $\text{PbCl}_2$  and  $\text{Pb}(\text{ClO}_4)_2$  were performed in RADCOR, RADPROF, and iFADO during 2018–2020 (Table 1).


The second major change in the methodology was proposed by SHA17, who recommended readjusting the measured  $R$  into an offset-corrected  $R^0$  (eq 5 and Appendix B). In this study, the proposed correction was implemented for the cruises where the SHI2600 spectrophotometer was used (Table 1). The equip-

ment was examined for potential wavelength accuracy offsets using a holmium oxide standard (type 667-UV5, provided by Hellma) to assess the  $\Delta\lambda_{241.1}$  term (eq 5). Lacking a detailed wavelength accuracy test procedure in SHA17, all the measurements were performed reproducing the calibration conditions described in the holmium certification. After 15 determinations, which yielded values between 0.1 nm and 0.3 nm,  $\Delta\lambda_{241.1}$  was assigned an average value of 0.2 nm, which equals the uncertainty of the certified peak. This offset was applied to  $R$  data from HOTMIX, MSM72, RADPROF, iFADO, and RADCOR (Table 1). The PE850 spectrophotometer was also examined during the iFADO cruise, with three determinations, yielding  $\Delta\lambda_{241.1}$  equal to zero. For the remaining cruises, we were unable to examine the equipment, or these had been recalibrated after the cruise; therefore, no wavelength offset correction was applied to CAIBOX, MOC2, OVIDE, TALPRO, and MEDWAVES. Small deviations from the reference temperature ( $25^\circ\text{C}$ ) were accounted for using SHA19 formulations since the temperature was measured for each sample (mean difference in temperature measurement with regard to  $25^\circ\text{C}$  ranged between  $0.02^\circ\text{C}$  and  $0.70^\circ\text{C}$  among data sets).

$R$  values obtained with  $\text{PbCl}_2$  and  $\text{Pb}(\text{ClO}_4)_2$  were indistinctly used with the different formulations in Tables S1 and S2 and  $[\text{CO}_3^{2-}]_{\text{spec}}$  were calculated using all possible combinations between formulations and reagents, under the following assumption: neither the molecular Pb(II) complex added nor its final concentration in the cuvette should affect the absorbance measurements since the method relies on the characterization of the Pb(II) absorbance signal in seawater.<sup>27</sup> This would be supported by the fact that PAT15 assessed the formulations by BY08 that were obtained with  $\text{PbCl}_2$  with data measured with  $\text{Pb}(\text{ClO}_4)_2$  and proposed using the same formulation for  $e_3/e_2$  as BY08 (Table S2). Hence, five different  $[\text{CO}_3^{2-}]_{\text{spec}}$  values were obtained for each measured  $R$  value. The BY08, EAS13, PAT15, and SHA17 formulations in Table S2 are referred to  $25^\circ\text{C}$  and atmospheric pressure, being a function of  $R$  and salinity. Only the formulation by SHA19 is also temperature-dependent. Hereafter, the particular  $[\text{CO}_3^{2-}]_{\text{spec}}$  is noted as  $[\text{CO}_3^{2-}]_{\text{spec}X}$ , where  $X$  is the approach abbreviation (BY08, EAS13, PAT15, SHA17, and SHA19).

Fajar et al.<sup>44</sup> reported  $[\text{CO}_3^{2-}]_{\text{spec}}$  data from the CAIBOX, MOC2, HOTMIX, and OVIDE cruises, comparing BY08 and EAS13 formulations. This study adds new  $[\text{CO}_3^{2-}]_{\text{spec}}$  data from six cruises in the Mediterranean Sea (TALPRO, MEDWAVES, and MSM72) and the northeast Atlantic Ocean (MEDWAVES, RADPROF, RADCOR, and iFADO). The compiled data cover a wide range of oceanographic conditions in terms of salinity ( $33.7\text{--}39.3$ ), pH ( $7.47$  pH units  $\text{--}8.13$  pH units), TA ( $2249 \mu\text{mol}\cdot\text{kg}^{-1}$   $\text{--}2639 \mu\text{mol}\cdot\text{kg}^{-1}$ ), TA/DIC ratio ( $1.02\text{--}1.18$ ), and the expected  $[\text{CO}_3^{2-}]$  ( $68 \mu\text{mol}\cdot\text{kg}^{-1}$   $\text{--}252 \mu\text{mol}\cdot\text{kg}^{-1}$ ) from coastal to open ocean. These ranges are mostly representative of typical open ocean surface conditions over the global ocean (Appendix A; Figure S1).

**2.2. Definition and Uncertainty in  $\Delta[\text{CO}_3^{2-}]$ .** The goodness of the five approaches for quantifying  $[\text{CO}_3^{2-}]_{\text{spec}}$  was evaluated in terms of the internal consistency between measured and calculated  $[\text{CO}_3^{2-}]$  following the works describing the methodology.<sup>24,25,28–30</sup> The internal consistency analysis assesses how well predicted values of  $[\text{CO}_3^{2-}]$  compare to the expected or reference  $[\text{CO}_3^{2-}]$  values. To this end,  $[\text{CO}_3^{2-}]$  residuals were obtained as the difference between measured  $[\text{CO}_3^{2-}]_{\text{spec}}$  and  $[\text{CO}_3^{2-}]$  calculated from thermodynamic equations with paired  $\text{CO}_2$  variables ( $[\text{CO}_3^{2-}]_{\text{calc}}$ )

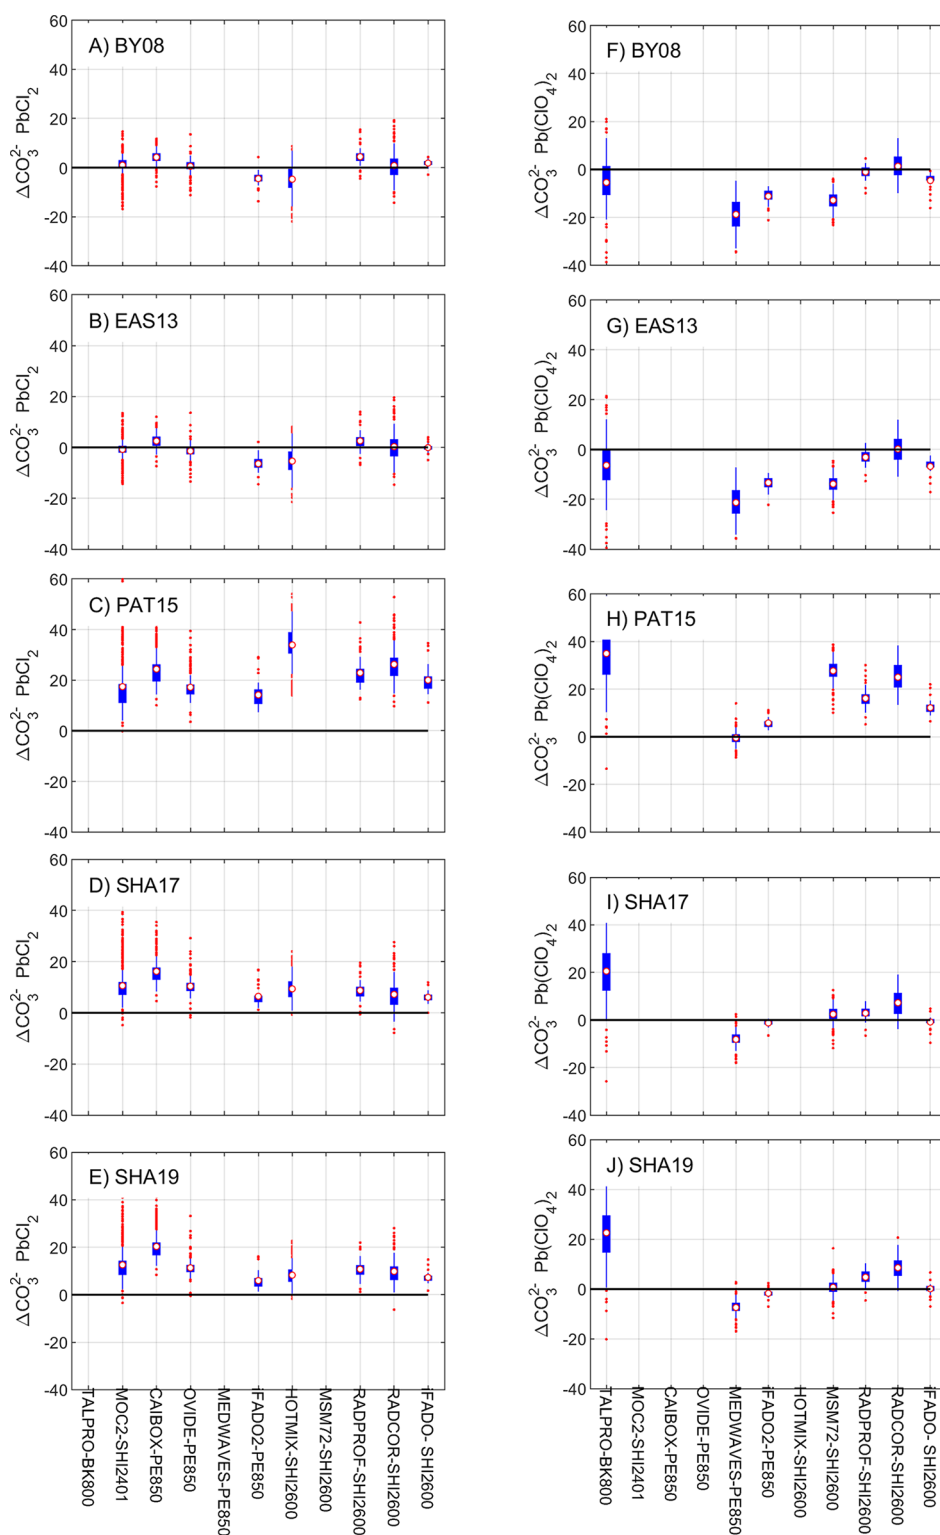

**Figure 2.** Whisker plots showing spectrophotometric minus calculated carbonate ion content ( $\Delta[\text{CO}_3^{2-}] = [\text{CO}_3^{2-}]_{\text{spec}} - [\text{CO}_3^{2-}]_{\text{calc}}$  in  $\mu\text{mol}\cdot\text{kg}^{-1}$ ) for cruises in Figure 1 and Table 1. The central dot denotes the mean  $\Delta[\text{CO}_3^{2-}]$ , and the lower and upper limits of the blue box are the first and third quartiles, respectively. Whiskers cover 95% of data variance. Red dots are outliers located beyond one-time the interquartile range.  $[\text{CO}_3^{2-}]_{\text{spec}}$  is obtained with five different formulations (Table S2): (A and F) BY08, (B and G) EAS13, (C and H) PAT15, (D and I) SHA17, and (E and J) SHA19. Left and right panels refer to  $[\text{CO}_3^{2-}]_{\text{spec}}$  data measured with  $\text{PbCl}_2$  and  $\text{Pb}(\text{ClO}_4)_2$ , respectively. The cruise alias and the spectrophotometer model used (Table 1) are indicated as x-axis labels.  $[\text{CO}_3^{2-}]_{\text{calc}}$  is calculated with pH-TA. Calculations are reported at 25 °C and atmospheric pressure except for SHA19 that are reported at the exact temperature of analysis. The SHA17 and SHA19 approaches include a wavelength correction ( $\Delta\lambda_{241.1} = 0.2$  nm, Table S1) for cruises where the SH12600 was used (HOTMIX, MSM72, RADPROF, RADCOR, and iFADO; Table 1) and is null for the remaining cruises.

( $\Delta[\text{CO}_3^{2-}] = [\text{CO}_3^{2-}]_{\text{spec}} - [\text{CO}_3^{2-}]_{\text{calc}}$  in  $\mu\text{mol}\cdot\text{kg}^{-1}$ ). Each of the five  $[\text{CO}_3^{2-}]_{\text{spec}}$  determinations was considered a predicted value, dependent on different sets of calibration functions (Table S2), to be compared to the expected  $[\text{CO}_3^{2-}]_{\text{calc}}$ .  $[\text{CO}_3^{2-}]_{\text{calc}}$  was considered the reference value because it is based on paired  $\text{CO}_2$  input variables that have solid SOPs, CRMs exist for some of them, and the methodology for measuring  $[\text{CO}_3^{2-}]_{\text{spec}}$  is itself defined according to  $[\text{CO}_3^{2-}]_{\text{calc}}$  (Appendixes B and D).<sup>24,25,28–30</sup> As for  $[\text{CO}_3^{2-}]_{\text{spec}}$ , corresponding  $\Delta[\text{CO}_3^{2-}]$  will be noted as  $\Delta[\text{CO}_3^{2-}]_X$ , where X is the approach abbreviation (BY08, EAS13, PAT15, SHA17, and SHA19).

$[\text{CO}_3^{2-}]_{\text{calc}}$  was estimated using the MATLAB CO2SYS software,<sup>45</sup> at 25 °C and atmospheric pressure, using both measured pH-TA and TA-DIC pairs, along with total phosphate and silicate. The  $\text{CO}_2$  equilibrium constants of Mehrbach et al.<sup>46</sup> reformulated on the total hydrogen scale by Lueker et al.<sup>47</sup> the bisulfate equilibrium constant of Dickson,<sup>48</sup> and the boron to chlorinity ratio of Lee et al.<sup>49</sup> were used for the calculations. Absolute differences between  $[\text{CO}_3^{2-}]_{\text{calc}}$  derived from TA-pH and TA-DIC were not significant (Appendix D). Since paired measurements of pH-TA are more abundant than TA-DIC pairs ( $N = 2367$  and  $N = 628$ , respectively),  $[\text{CO}_3^{2-}]_{\text{calc}}$  results shown refer to  $[\text{CO}_3^{2-}]_{\text{calc}}$  from pH and TA.

Studying the internal consistency of  $\Delta[\text{CO}_3^{2-}]$  implies studying how well each of the five predicted values of  $[\text{CO}_3^{2-}]_{\text{spec}}$ , dependent on different sets of coefficients (Table S2), compare with the expected  $[\text{CO}_3^{2-}]_{\text{calc}}$  within given limits of uncertainty. A limit of uncertainty of  $\pm 4\%$  of the expected  $[\text{CO}_3^{2-}]_{\text{calc}}$  was obtained by propagating the standard uncertainties of  $[\text{CO}_3^{2-}]_{\text{spec}}$  and  $[\text{CO}_3^{2-}]_{\text{calc}}$ . For  $[\text{CO}_3^{2-}]_{\text{spec}}$ , the value of  $\pm 2\%$  standard uncertainty, assigned among approaches (Table S1 and Appendix C), was considered. The total standard uncertainty of  $[\text{CO}_3^{2-}]_{\text{calc}}$  was calculated using the software package *errors* from Orr et al.<sup>37</sup> (Appendix D). For the calculations, the following uncorrelated uncertainties were assigned to the input  $\text{CO}_2$  system variables:  $\pm 0.01$  pH units for pH,  $\pm 3 \mu\text{mol}\cdot\text{kg}^{-1}$  for TA (section 2.1), and the uncertainty for the equilibrium constants was taken from Table 1 in Orr et al.<sup>37</sup> Ancillary variables (temperature, salinity, and pressure) and inorganic nutrients were assumed to have negligible standard uncertainty, as in SHA19. The resulting total uncertainty is proportional to  $[\text{CO}_3^{2-}]_{\text{calc}}$  and ranges between  $2.5 \mu\text{mol}\cdot\text{kg}^{-1}$  and  $8 \mu\text{mol}\cdot\text{kg}^{-1}$  ( $\pm 3.2\% - \pm 3.7\%$ ) for the studied  $[\text{CO}_3^{2-}]_{\text{calc}}$  range ( $68 \mu\text{mol}\cdot\text{kg}^{-1}$  to  $252 \mu\text{mol}\cdot\text{kg}^{-1}$ ) (Appendix D; Figure S4). The resulting propagated uncertainty limit to consider  $\Delta[\text{CO}_3^{2-}]$  internally consistent within the  $[\text{CO}_3^{2-}]_{\text{calc}}$  range in this study ranged from  $\pm 3.8\%$  to  $\pm 4.2\%$  and was averaged to  $\pm 4\%$ .

Internally consistent  $\Delta[\text{CO}_3^{2-}]$  values will distribute randomly around zero until the  $\pm 4\%$  limit. Larger  $\Delta[\text{CO}_3^{2-}]$  values might be due to particularities of each approach, either relative to the respective calibration functions fitting conditions or to the differing methodological recommendations for obtaining *R* values (Table S1). This limit also allows assessing whether there is internal consistency across the five  $[\text{CO}_3^{2-}]_{\text{spec}}$  determinations. Note that the choice of the pH-TA pair implies a more conservative interpretation of the  $\Delta[\text{CO}_3^{2-}]$  with regard to the TA-DIC pair because of the larger uncertainty in  $[\text{CO}_3^{2-}]_{\text{calc}}$  (Appendix D) and is based on assuming quite large uncertainties in the input variables. In addition,  $\Delta[\text{CO}_3^{2-}]$  are also evaluated according to the standard uncertainty limits for weather and climate-quality objectives for OA studies

recommended by the Global Ocean Acidification Observing Network (GOA-ON)<sup>50</sup> of  $\pm 10\%$  and  $\pm 1\%$ , respectively.

### 3. RESULTS

**3.1. Overview of  $\Delta[\text{CO}_3^{2-}]$  Results.** Figure 2 shows an overview of the  $\Delta[\text{CO}_3^{2-}]$  results by approach, reagent, cruise, and spectrophotometer (values in Table S4). BY08 and EAS13 formulations yield  $\Delta[\text{CO}_3^{2-}]$  close to zero or negative, while the formulations of PAT15, SHA17, and SHA19 yield overall positive  $\Delta[\text{CO}_3^{2-}]$ , particularly PAT15. Regardless of the Pb(II) reagent,  $\Delta[\text{CO}_3^{2-}]$  among the five approaches always distribute the same way:  $\Delta[\text{CO}_3^{2-}]_{\text{EAS13}}$  and  $\Delta[\text{CO}_3^{2-}]_{\text{BY08}}$  are comparable and usually show lower values than  $\Delta[\text{CO}_3^{2-}]_{\text{SHA17}}$  and  $\Delta[\text{CO}_3^{2-}]_{\text{SHA19}}$  that are also comparable, while  $\Delta[\text{CO}_3^{2-}]_{\text{PAT15}}$  shows the highest positive values. In particular, one distinct feature between reagents is that *R* data obtained with  $\text{PbCl}_2$  show larger dispersion and more outliers (red dots) than  $\text{Pb}(\text{ClO}_4)_2$  data.


$\Delta[\text{CO}_3^{2-}]_{\text{BY08}}$  and  $\Delta[\text{CO}_3^{2-}]_{\text{EAS13}}$  show mean values close to zero and mostly comprised within the  $\pm 4\%$  limit for Atlantic Ocean cruises (CAIBOX, MOC2, OVIDE, RADPROF, RADCOR, and iFADO) and one Mediterranean Sea cruise (TALPRO) (Figure 2; Table S4), regardless of the Pb(II) reagent. Negative values beyond the  $\pm 4\%$  limit are found for one cruise in the Atlantic Ocean (iFADO), two cruises in the Mediterranean Sea (HOTMIX and MSM72), and in regions influenced by Mediterranean waters (MEDWAVES), especially for  $\text{Pb}(\text{ClO}_4)_2$  data (Figure 2; Table S4).

Clearly,  $\Delta[\text{CO}_3^{2-}]_{\text{PAT15}}$  shows the largest positive values, mostly above the  $\pm 10\%$  limit for data from either Pb(II) reagent, except for the MEDWAVES cruise that shows  $\Delta[\text{CO}_3^{2-}]_{\text{PAT15}}$  centered around zero (Figure 2; Table S4).  $\Delta[\text{CO}_3^{2-}]_{\text{SHA17}}$  and  $\Delta[\text{CO}_3^{2-}]_{\text{SHA19}}$  yield mainly positive values between the  $\pm 4\%$  and  $\pm 10\%$  limits (Table S4). The SHA17 and SHA19 approaches overall show comparable results, which is expected since all the measurements were performed at 25 °C. These results support the consistency between the SHA17 and SHA19 approaches when the measurements are performed at the same temperature, and differences between them might be due to biases from the reference temperature during analysis (section 2.1), which can be accounted for with the SHA19 approach.

The approaches of SHA17 and SHA19 propose a correction (eq 5) to account for wavelength inaccuracies in the spectrophotometer. In this regard,  $\Delta[\text{CO}_3^{2-}]_{\text{SHA17}}$  and  $\Delta[\text{CO}_3^{2-}]_{\text{SHA19}}$  from measurements obtained with the SHI2600 spectrophotometer (HOTMIX, MSM72, RADPROF, RADCOR, and iFADO) showed positive values that decreased and approached zero after applying the measured  $\Delta\lambda_{241.1}$  term for data from either Pb(II) reagent (Figure 2). However, Figure 2 shows that final readjusted  $\Delta[\text{CO}_3^{2-}]_{\text{SHA17}}$  and  $\Delta[\text{CO}_3^{2-}]_{\text{SHA19}}$  do not center completely around zero for some of these cruises (HOTMIX, RADPROF, and RADCOR). The PE850 spectrophotometer could only be examined during iFADO, for which  $\Delta\lambda_{241.1}$  was zero, and corresponding  $\Delta[\text{CO}_3^{2-}]_{\text{SHA17}}$  and  $\Delta[\text{CO}_3^{2-}]_{\text{SHA19}}$  are well centered around zero only for data measured with  $\text{Pb}(\text{ClO}_4)_2$  (Figure 2; Table S4). The  $\Delta[\text{CO}_3^{2-}]$  for the cruises for which the  $\Delta\lambda_{241.1}$  term could not be measured (CAIBOX, MOC2, OVIDE, TALPRO, and MEDWAVES) approached zero if *R* was readjusted using a  $\Delta\lambda_{241.1}$  value of about 0.3 nm (results not shown).

**3.2. Patterns in  $\Delta[\text{CO}_3^{2-}]$  versus  $[\text{CO}_3^{2-}]_{\text{calc}}$ .** The magnitude of  $\Delta[\text{CO}_3^{2-}]$  is proportional to  $[\text{CO}_3^{2-}]_{\text{calc}}$  itself,



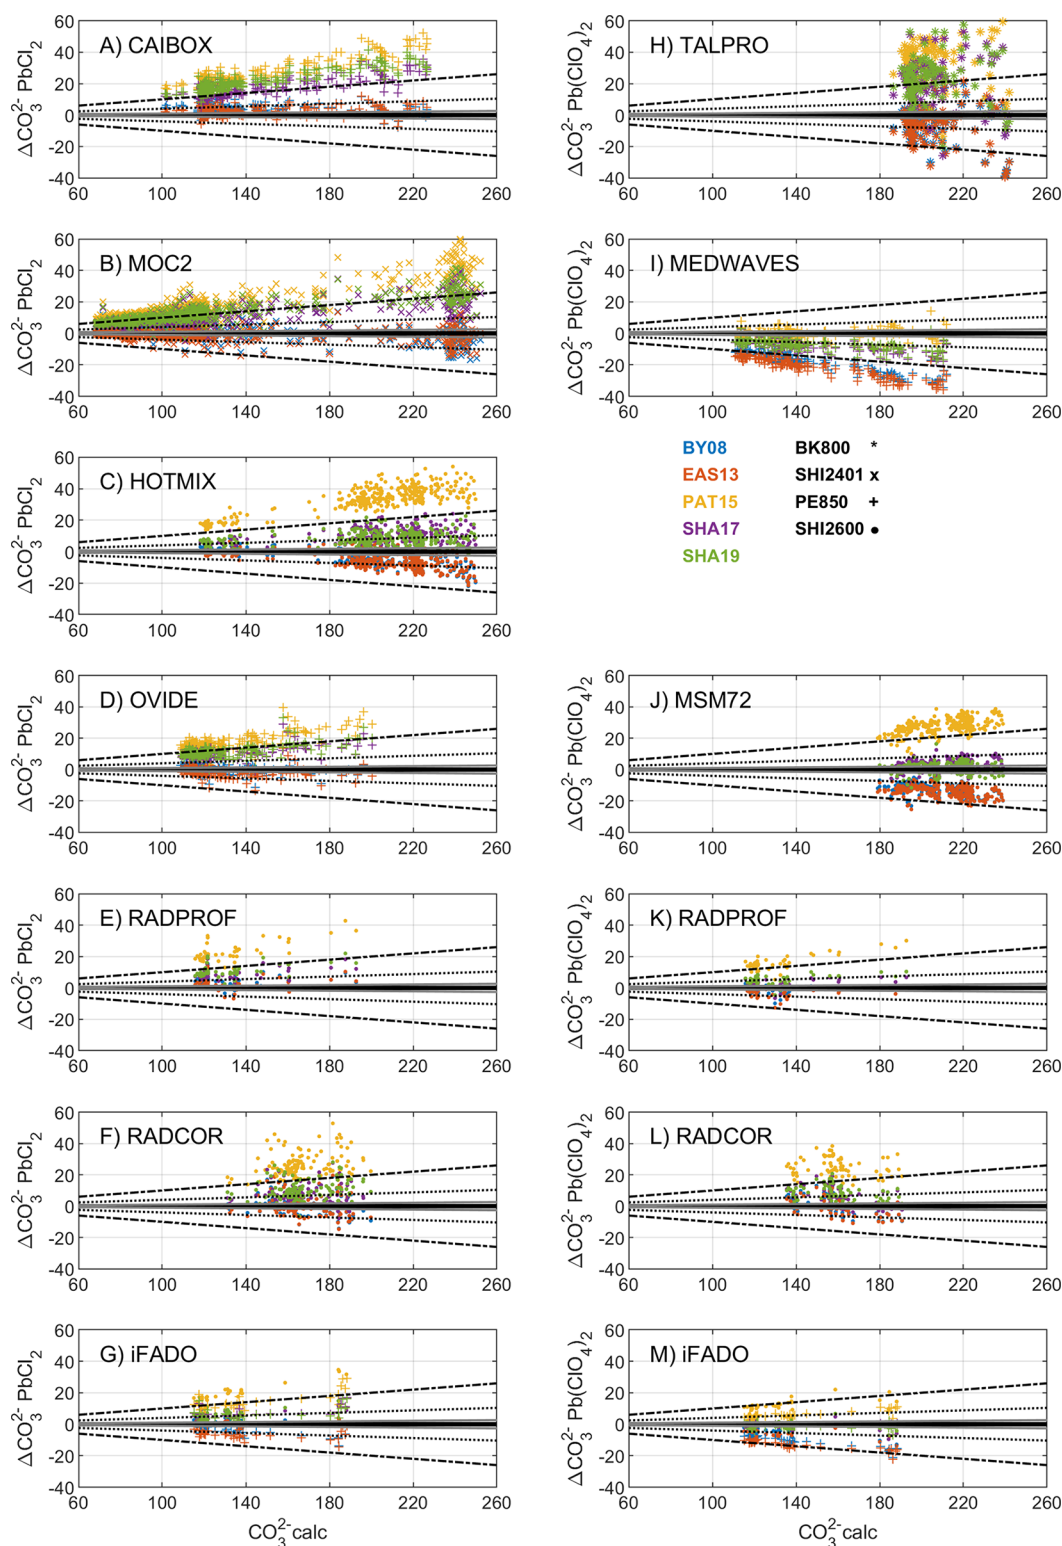

**Figure 3.** Spectrophotometric minus calculated carbonate ion content ( $\Delta[\text{CO}_3^{2-}] = [\text{CO}_3^{2-}]_{\text{spec}} - [\text{CO}_3^{2-}]_{\text{calc}}$ ; in  $\mu\text{mol}\cdot\text{kg}^{-1}$ ) as a function of  $[\text{CO}_3^{2-}]_{\text{calc}}$  (calculated from pH-TA;  $\mu\text{mol}\cdot\text{kg}^{-1}$ ) for each cruise (Figure 1; Table 1).  $[\text{CO}_3^{2-}]_{\text{spec}}$  are obtained with five  $[\text{CO}_3^{2-}]_{\text{spec}}$  formulations (Table S1) in color. Spectrophotometer models (Table S3) are identified with different symbols. Panels on the left and the right refer to  $[\text{CO}_3^{2-}]_{\text{spec}}$  data measured with  $\text{PbCl}_2$  and  $\text{Pb}(\text{ClO}_4)_2$ , respectively.  $[\text{CO}_3^{2-}]_{\text{calc}}$  are reported at 25 °C and atmospheric pressure, except for SHA19 that are reported at the exact temperature of analysis. The SHA17 and SHA19 approaches include a wavelength correction ( $\Delta\lambda_{241.1} = 0.2 \text{ nm}$ ; Table S1) for cruises where the SHI2600 was used (HOTMIX, MSM72, RADPROF, RADCOR, and iFADO; Table 1) and is null for the remaining cruises. Gray and dashed lines depict the GOA-ON relative standard uncertainty goals of  $\pm 1\%$  for the climate-quality objective and  $\pm 10\%$  for the weather-quality objective, respectively; the dotted line depicts the standard uncertainty limit of  $\pm 4\%$  attributable to the internal consistency of the data set in this study.

as reported in all the works of the methodology,<sup>24,25,28–30,44</sup> regardless of the Pb(II) reagent, the spectrophotometer, or the approach used (Figure 3). The approaches by BY08 and EAS13 yield  $\Delta[\text{CO}_3^{2-}]$  that mostly scatter around zero (CAIBOX, MOC2, and OVIDE) except for Mediterranean Sea cruises (i.e., high-salinity waters; HOTMIX, MSM72, MEDWAVES, and TALPRO) and for the iFADO cruise, where  $\Delta[\text{CO}_3^{2-}]_{\text{BY08}}$  and  $\Delta[\text{CO}_3^{2-}]_{\text{EAS13}}$  show negative values that decrease towards higher  $[\text{CO}_3^{2-}]_{\text{calc}}$  (i.e., increasing  $[\text{CO}_3^{2-}]_{\text{spec}}$  underestimation). The approaches by PAT15, SHA17, and SHA19 show the opposite  $\Delta[\text{CO}_3^{2-}]$  patterns, with  $\Delta[\text{CO}_3^{2-}]_{\text{PAT15}}$ ,  $\Delta[\text{CO}_3^{2-}]_{\text{SHA17}}$ , and  $\Delta[\text{CO}_3^{2-}]_{\text{SHA19}}$  that increase proportionally to  $[\text{CO}_3^{2-}]_{\text{calc}}$  (i.e., increasing  $[\text{CO}_3^{2-}]_{\text{spec}}$  overestimation). Figure 3 shows that the same relative distribution among  $\Delta[\text{CO}_3^{2-}]$  from each approach is observed for the whole  $[\text{CO}_3^{2-}]_{\text{calc}}$  range, where  $\Delta[\text{CO}_3^{2-}]_{\text{EAS13}} \approx \Delta[\text{CO}_3^{2-}]_{\text{BY08}} < \Delta[\text{CO}_3^{2-}]_{\text{SHA17}} \approx \Delta[\text{CO}_3^{2-}]_{\text{SHA19}} < \Delta[\text{CO}_3^{2-}]_{\text{PAT15}}$ , as reported in section 3.1. This pattern between approaches was expected for the whole  $[\text{CO}_3^{2-}]_{\text{calc}}$  range at salinity 35, as shown in Figure S2A. It is attributable to differences among calibration functions (Table S2) that are larger at low  $R$  values (i.e., higher  $[\text{CO}_3^{2-}]_{\text{calc}}$ ; Figure S2) and higher salinities (Figure S3).

The spectrophotometer used affects the dispersion (Appendix C) in  $\Delta[\text{CO}_3^{2-}]$  (Figure 3). For instance, data from the TALPRO cruise show larger  $\Delta[\text{CO}_3^{2-}]$  dispersion and also larger whisker boxes than other cruises (Figure 2). During TALPRO,  $[\text{CO}_3^{2-}]_{\text{spec}}$  values were measured with a BK800 spectrophotometer (Table 1), which is a single beam and also the least accurate spectrophotometer of all the models used in terms of photometric accuracy (Appendix C; Table S3). In contrast, cruises using the PE850 spectrophotometer (CAIBOX, MEDWAVES, OVIDE, and iFADO) show the lowest  $\Delta[\text{CO}_3^{2-}]$  dispersion for the entire  $[\text{CO}_3^{2-}]_{\text{calc}}$  range (Figure 3). This spectrophotometer has the best photometric accuracy and also a very low value for stray light (Table S3). Between them, in terms of photometric accuracy performance, the SHI2401 and SHI2600 models (Table S3) yield data with increasing dispersion toward higher  $[\text{CO}_3^{2-}]_{\text{calc}}$  for cruises where  $[\text{CO}_3^{2-}]_{\text{calc}} > 180 \mu\text{mol}\cdot\text{kg}^{-1}$  (MOC2, HOTMIX, and MSM72). The larger dispersion for RADCOR over the entire  $[\text{CO}_3^{2-}]_{\text{calc}}$  range might be related to being a coastal site with higher inherent variability.<sup>7</sup>

Also, the spectrophotometer used affects the overall bias (Appendix C) in  $\Delta[\text{CO}_3^{2-}]$ . PE850 exemplifies well that highly precise equipment in terms of dispersion (i.e., photometric accuracy; Table S3) can exhibit very different performance in terms of bias (i.e., wavelength accuracy; CAIBOX, MEDWAVES, OVIDE, and iFADO; Figure 3). In this regard, since  $\Delta[\text{CO}_3^{2-}]$  from each of the five approaches always keep the same relationship among them, the approaches that respectively show the most internally consistent  $\Delta[\text{CO}_3^{2-}]$ , within the  $\pm 4\%$  limit of  $[\text{CO}_3^{2-}]_{\text{calc}}$  are cruise-dependent, in relation to the spectrophotometer bias: SHA17 and SHA19 (MSM72, Pb( $\text{ClO}_4$ )<sub>2</sub>; iFADO, both reagents), EAS13 and BY08 (CAIBOX, MOC2, and OVIDE, all using PbCl<sub>2</sub>; RADPROF and RADCOR, both reagents), and PAT15 (MEDWAVES, Pb( $\text{ClO}_4$ )<sub>2</sub>).

**3.3. Limits of Consistency for  $\Delta[\text{CO}_3^{2-}]$ .** No approach fulfills the GOA-ON relative standard uncertainty goal of  $\pm 1\%$  for the climate-quality objective, but most results, except those obtained with the PAT15 approach, meet the weather-quality objective of  $\pm 10\%$  uncertainty for any range of  $[\text{CO}_3^{2-}]_{\text{calc}}$  (Figure 3; Table S5).

Cruises in the Atlantic Ocean, except the iFADO cruise, show  $\Delta[\text{CO}_3^{2-}]$  values within  $\pm 4\%$  uncertainty with the BY08 and EAS13 approaches for the whole  $[\text{CO}_3^{2-}]_{\text{calc}}$  range (Figure 3; Table S5). Hence,  $[\text{CO}_3^{2-}]_{\text{specBY08}}$  or  $[\text{CO}_3^{2-}]_{\text{specEAS13}}$  are internally consistent within the assumed uncertainty (Section 2.2). This was already reported by Fajar et al.<sup>44</sup> for the Atlantic Ocean data (CAIBOX, MOC2, and OVIDE). Although the EAS13 approach was reported to be accurate enough ( $\pm 2\%$ ) only below  $180 \mu\text{mol}\cdot\text{kg}^{-1}$  by PAT15,<sup>29</sup> the results in this study suggest that both BY08 and EAS13 formulations determine consistent  $[\text{CO}_3^{2-}]_{\text{spec}}$  ( $\pm 4\%$ ) in the North Atlantic Ocean, over the  $68 \mu\text{mol}\cdot\text{kg}^{-1} - 252 \mu\text{mol}\cdot\text{kg}^{-1}$  range.


For high-salinity waters, the BY08 and EAS13 approaches yield mostly negative  $\Delta[\text{CO}_3^{2-}]$  (although still within  $\pm 4\%$  when using PbCl<sub>2</sub> (HOTMIX)) that show larger  $\Delta[\text{CO}_3^{2-}]$  (within  $\pm 10\%$  or beyond) when using Pb( $\text{ClO}_4$ )<sub>2</sub> (TALPRO, MEDWAVES, and MSM72; Table S5). The EAS13 approach was reported to underestimate  $[\text{CO}_3^{2-}]_{\text{spec}}$  at salinity  $> 36$ ,  $[\text{CO}_3^{2-}]_{\text{calc}} > 150 \mu\text{mol}\cdot\text{kg}^{-1}$ , and high pH.<sup>28,44</sup> This study shows that the underestimation of  $[\text{CO}_3^{2-}]_{\text{spec}}$  occurs for the HOTMIX, MEDWAVES, and MSM72 cruises, with the BY08 and EAS13 approaches. In this regard, EAS13 suggested that the Pb(II) complexation model should be extended to include the formation of other potential Pb(II) complexes to address the trend in the residuals seen at high  $[\text{CO}_3^{2-}]$  (Appendix B). However, opposite to the approaches of BY08 and EAS13, the most recent approaches of SHA17 and SHA19, with the latter covering a wide salinity fitting range (Table S1), do not underestimate  $[\text{CO}_3^{2-}]_{\text{spec}}$ ; yet, in some cruises overestimate it (Figure 3; Table S5). Hence, the hypothesis of a mischaracterization of the Pb(II) complexation in high-salinity and high-pH waters would not be supported. Instead, the fitting procedure for the terms in eq 1 for each approach might cause the observed negative  $\Delta[\text{CO}_3^{2-}]$ , as the greatest changes regarding the stability constant for the formation of the PbCO<sub>3</sub> complex (Figure S2B) and the terms  $\left[\frac{1}{R - \epsilon_1}\right]$  and  $\left[1 - R \cdot \frac{\epsilon_3}{\epsilon_2}\right]$  (Figure S3) were mostly generated for high-salinity and low  $R$  values.

## 4. DISCUSSION


Both the observed mean  $\Delta[\text{CO}_3^{2-}]$  values and corresponding trends versus  $[\text{CO}_3^{2-}]_{\text{calc}}$ , taking into account reagents, equipment specifications and calibration, salinity ranges, and  $[\text{CO}_3^{2-}]_{\text{calc}}$ , suggest that the method is inconsistent among approaches with regard to its performance for  $[\text{CO}_3^{2-}]_{\text{spec}}$  measurement. In this section, the methodological changes among approaches are assessed to identify the factors that explain the observed differences in  $\Delta[\text{CO}_3^{2-}]$ .

**4.1. Random and Systematic Uncertainty of the Absorbance Ratio ( $R$ ): Precision and Accuracy of Absorbance Measurements.** Since  $R$  values are inversely proportional to  $[\text{CO}_3^{2-}]_{\text{spec}}$  (i.e., lower  $R$  values yield higher  $[\text{CO}_3^{2-}]_{\text{spec}}$ ; Figure S2A inset), the assessment of  $[\text{CO}_3^{2-}]_{\text{spec}}$  is less precise at a higher  $[\text{CO}_3^{2-}]$ , and this is independent of the equipment or approach used. Within  $R$  (eq 2),  $_{250A}$  varies substantially with pH,<sup>24,27,33</sup> becoming lower as  $[\text{CO}_3^{2-}]$  increases, while  $_{234A}$  is always higher, lying close to the isosbestic point (Appendix C) and is thus less sensitive to changes in  $[\text{CO}_3^{2-}]$ . In consequence, lower  $R$  values will inherently have larger random uncertainty, or lower precision, which translates into a fan-shape distribution of  $\Delta[\text{CO}_3^{2-}]$  for results obtained with any approach, particularly at  $[\text{CO}_3^{2-}]_{\text{calc}} > 180 \mu\text{mol}\cdot\text{kg}^{-1}$  (Figure 3). This fact, derived from  $R$  being a ratio of absorbances



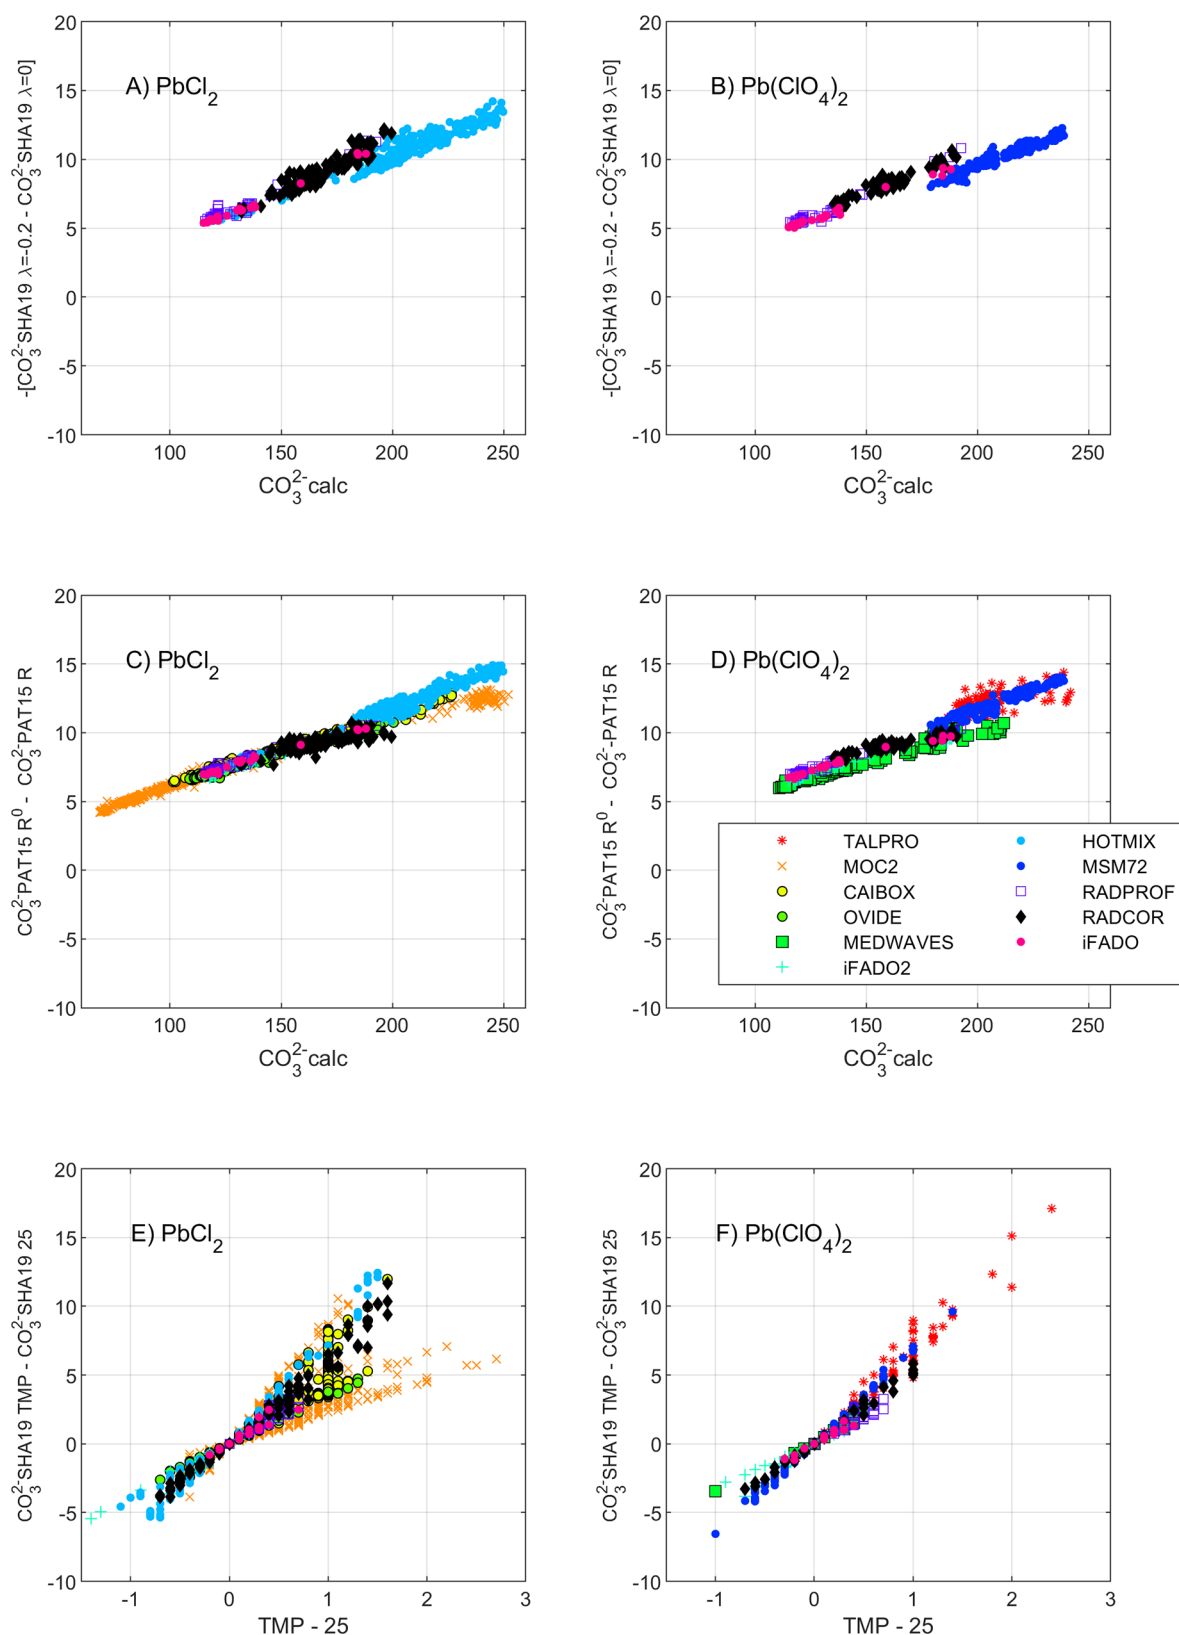

**Figure 4.** Effect on  $[\text{CO}_3^{2-}]_{\text{spec}}$  (in  $\mu\text{mol}\cdot\text{kg}^{-1}$ ) of (A and B) the wavelength offset correction proposed by SHA17 as a function of  $[\text{CO}_3^{2-}]_{\text{calc}}$  (calculated from TA-pH;  $\mu\text{mol}\cdot\text{kg}^{-1}$ ), (C and D) the Pb(II) reagent perturbation correction according to PAT15 as a function of  $[\text{CO}_3^{2-}]_{\text{calc}}$  and (E and F) the functions proposed by SHA19 as a function of the temperature bias regarding 25 °C. Differences are calculated as (A and B)  $[\text{CO}_3^{2-}]_{\text{spec}}$  calculated using a wavelength offset correction ( $\Delta\lambda_{241.1}$ ) of 0.2 nm (eq 4) minus  $[\text{CO}_3^{2-}]_{\text{spec}}$  obtained without correction, for cruises using the SHI2600 spectrophotometer; (C and D)  $[\text{CO}_3^{2-}]_{\text{spec}}$  calculated with the corrected minus the original Pb(II) absorbance ratio ( $R^0$  and  $R$ , respectively; Table S1); (E and F)  $[\text{CO}_3^{2-}]_{\text{spec}}$  at the real temperature (TMP) of analysis minus  $[\text{CO}_3^{2-}]_{\text{spec}}$  at 25 °C. Data measured with  $\text{PbCl}_2$  or  $\text{Pb}(\text{ClO}_4)_2$  are shown on the left and the right panels, respectively. All panels share the same legend.

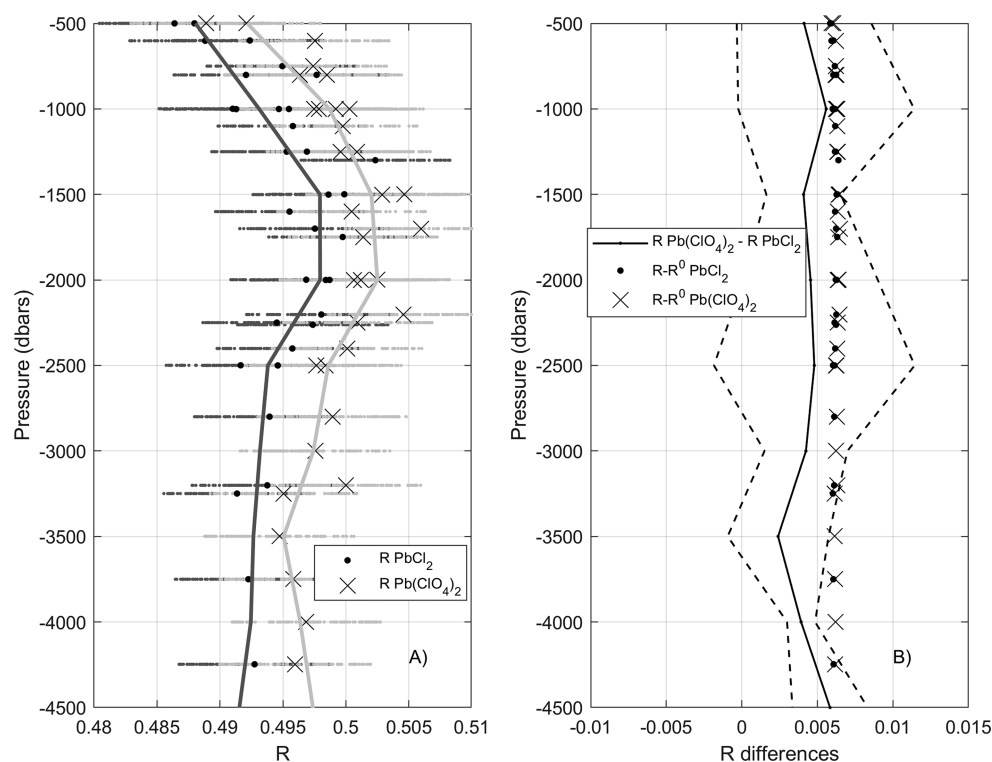

**Figure 5.** (A) Mean profiles of Pb(II) absorbance ratios ( $R$ ) for sample replicates measured with  $\text{PbCl}_2$  (dark line and dots) and  $\text{Pb}(\text{ClO}_4)_2$  (gray line and crosses) during the RADPROF cruise (Table 1). Horizontal dotted lines accompanying each  $R$  value correspond to a Monte Carlo perturbation analysis introducing a random uncertainty within  $\pm 0.006$  in measured  $R$  values according to SHI2600 specifications (Table S3). (B) Mean difference profile of  $R$  measured with  $\text{Pb}(\text{ClO}_4)_2$  minus  $R$  measured with  $\text{PbCl}_2$  (solid line) and corresponding uncertainty (dashed lines) calculated considering the Monte Carlo perturbed  $R$  results shown in panel A. Additionally, the value of the  $R$  perturbation correction according to PAT15 ( $R^0 - R$ ; Table S1), for RADPROF replicate measurements with  $\text{PbCl}_2$  (dark dots) and  $\text{Pb}(\text{ClO}_4)_2$  (gray crosses) is also depicted. The sign of the perturbation values has been reversed for representation purposes.

with dissimilar magnitudes, can be empirically evidenced using a Monte Carlo analysis (Appendix E; Figure S5).

Technical specifications of the spectrophotometer regarding the photometric and wavelength accuracies, and the stray light (Table S3) might be critical for setting the mean  $\Delta[\text{CO}_3^{2-}]$  value and its relationship to  $[\text{CO}_3^{2-}]_{\text{calc}}$ . In this study, the spectrophotometers used have variable values for photometric accuracy (Appendix C), which translates into variable  $R$  uncertainty (Table S3) that will affect  $\Delta[\text{CO}_3^{2-}]$  to a different extent but always cause the same distribution (Figure S5). A spectrophotometer with low photometric accuracy will introduce more random noise in  $R$  measurements, especially at low  $R$  values, resulting in even more dispersed  $\Delta[\text{CO}_3^{2-}]$  at high  $[\text{CO}_3^{2-}]$ . Another factor affecting random uncertainty might be the stray light of the spectrophotometer (Appendix C). By combining both random sources of uncertainty and according to the spectrophotometers specifications (Table S3), the spectrophotometer models could be ordered from the highest to the lowest expected precision as PE850, SHI2600, SHI2401, and BK800, which agrees with the observed results (Figure 3; Tables S4 and S5).

While random uncertainty in  $R$  explains the larger dispersion of  $\Delta[\text{CO}_3^{2-}]$  at high  $[\text{CO}_3^{2-}]$ , it does not explain systematic biases in  $\Delta[\text{CO}_3^{2-}]$  toward positive or negative values outside the  $\pm 4\%$  limit (Figure 3). The wavelength accuracy is critical in this regard (Appendix C) since it could be significant when measuring  $_{250}\text{A}$ , located on a slope, where small variations in wavelength cause significant changes in  $_{250}\text{A}$ , and to a lesser extent in  $_{234}\text{A}$ , located near a peak. This was accounted for in

SHA17, who proposed a wavelength offset term ( $\Delta\lambda_{241.1}$ ; eq 5) to correct inaccuracies in the equipment wavelength calibration.

In this regard, measuring the holmium oxide standard to assess  $\Delta\lambda_{241.1}$  for the SHI2600 spectrophotometer was not simple. The  $\Delta\lambda_{241.1}$  term is supposed to remain constant as long as the equipment is not recalibrated.<sup>30</sup> However, 15  $\Delta\lambda_{241.1}$  measurements were averaged to obtain a stable value (section 2.1). Our experience quantifying  $\Delta\lambda_{241.1}$  indicates that (i) according to SHA17, shifts in  $\Delta\lambda_{241.1}$  on the order of 0.05 nm are supposed to be significant, which would imply that the holmium standard should be measured each time that the spectrophotometer is used, not only when recalibrated, because differences of this order were found for measurements of the same holmium oxide standard in different measurement exercises; (ii) the average  $\Delta\lambda_{241.1}$  found for SHI2600 ( $0.20 \text{ nm} \pm 0.06 \text{ nm}$ ) is lower than the wavelength accuracy of the spectrophotometer ( $\pm 0.3 \text{ nm}$ ; Table S3), and (iii) the average  $\Delta\lambda_{241.1}$  equals the uncertainty of the certified holmium peak position ( $241.15 \text{ nm} \pm 0.20 \text{ nm}$ ). Therefore,  $R$  measurements are likely corrected over the limits of the SHI2600 spectrophotometer and holmium standard specifications. However, when the offset correction is applied,  $\Delta[\text{CO}_3^{2-}]_{\text{SHA19}}$  decrease proportionally to  $[\text{CO}_3^{2-}]_{\text{calc}}$  by about  $5 \mu\text{mol}\cdot\text{kg}^{-1}$  to  $14 \mu\text{mol}\cdot\text{kg}^{-1}$ , for measurements with both reagents (Figure 4A, B). The SHA19 approach also uses  $\Delta\lambda_{241.1}$ . Despite adding complexity to the analysis procedure, both  $\Delta[\text{CO}_3^{2-}]_{\text{SHA17}}$  and  $\Delta[\text{CO}_3^{2-}]_{\text{SHA19}}$  meet the  $\pm 4\%$  uncertainty limit (Tables S3 and S4) and can be considered internally consistent, when the  $\Delta\lambda_{241.1}$  term is assessed, with the HOTMIX and RADCOR exceptions.

Technical specifications of the spectrophotometer seem crucial for precise and accurate  $R$  measurements. Most equipment might not achieve the accuracy necessary for  $[\text{CO}_3^{2-}]_{\text{spec}}$  determination (Table S3), including the model UV8453 used for describing the methodology (Table 1).<sup>30</sup> An accurate quantification of  $e_3/e_2$  and the fitting of  $\frac{\text{CO}_3\beta}{e_2}$  and  $e_1$  in eq 1 would benefit from using the best equipment in terms of technical specifications.

**4.2. Change in Pb(II) Reagent and Double Addition Correction.** PAT15 proposed a change in the Pb(II) reagent, from  $\text{PbCl}_2$  to  $\text{Pb}(\text{ClO}_4)_2$ , doubling the final Pb(II) concentration in the cuvette (Table S1), to increase the signal-to-noise ratio of the absorbance measurements. Additionally, the authors proposed an  $R$  perturbation correction (eq 4) that enlarges the resulting  $[\text{CO}_3^{2-}]_{\text{specPAT15}}$  proportionally to  $[\text{CO}_3^{2-}]_{\text{calc}}$  by  $5 \mu\text{mol}\cdot\text{kg}^{-1}$  to  $15 \mu\text{mol}\cdot\text{kg}^{-1}$  with regard to uncorrected  $R$  values (Figure 4C, D). As a result,  $\Delta[\text{CO}_3^{2-}]_{\text{PAT15}}$  values reach  $20 \mu\text{mol}\cdot\text{kg}^{-1}$  –  $40 \mu\text{mol}\cdot\text{kg}^{-1}$  at higher  $[\text{CO}_3^{2-}]_{\text{calc}}$  (Figure 3). If the correction is not applied,  $\Delta[\text{CO}_3^{2-}]_{\text{PAT15}}$  compares well with  $\Delta[\text{CO}_3^{2-}]_{\text{SHA17}}$  and  $\Delta[\text{CO}_3^{2-}]_{\text{SHA19}}$  (data not shown), which confirms that the large positive  $\Delta[\text{CO}_3^{2-}]_{\text{PAT15}}$  values are mainly caused by the perturbation correction. In this regard, no  $R$  perturbation correction was reported by BY08 or EAS13 for  $\text{PbCl}_2$  since the Pb(II) concentration in the cuvette ( $7.5 \mu\text{mol}\cdot\text{L}^{-1}$ ; Table S1) does not induce significant sample perturbation.<sup>28</sup> Neither of the most recent procedures by SHA17 and SHA19 recommends using a perturbation correction for  $R$  values measured with  $\text{Pb}(\text{ClO}_4)_2$ .

During the RADPROF cruise,  $R$  values were measured on replicate samples with  $\text{PbCl}_2$  and  $\text{Pb}(\text{ClO}_4)_2$  with the SHI2600 spectrophotometer (Table 1). The same comparison experiment was repeated during the iFADO cruise, where two different spectrophotometers were used: SHI2600 and PE850 (Table 1). RADPROF results reveal that  $R$  values measured with  $\text{Pb}(\text{ClO}_4)_2$  are higher than those measured with  $\text{PbCl}_2$  (Figure 5A) for sample replicates. The difference is almost constant for the whole depth profile and amounts to  $0.0044 \pm 0.0010$  ( $\text{Pb}(\text{ClO}_4)_2 - \text{PbCl}_2$ ; Figure 5B). Noticeably, the two reagents might behave differently characterizing the Pb(II) absorbance signal for the same seawater conditions. Considering a random uncertainty of  $\pm 0.006$  (Table S3) in  $R$  measurements, according to SHI2600 specifications, the mean  $R$  difference found between reagents is close to the  $R$  random uncertainty. In this regard, a Monte Carlo experiment introducing this random noise in the bulk  $R$  data from both reagents shows that resulting  $R$  values overlap (Figure 5A). This overlapping is magnified for spectrophotometers with lower photometric accuracy (data not shown). This would explain the absence of a significant difference of mean  $\Delta[\text{CO}_3^{2-}]$  using either reagent and formulations (Figure 2 and Table S4). In addition, Figure 5B shows that the observed  $R$  difference between reagents has almost the same magnitude but opposite sign to the magnitude of the  $R$  perturbation correction proposed by PAT15 ( $-0.006 \pm 0.0005$ ) for data measured using  $\text{PbCl}_2$  or  $\text{Pb}(\text{ClO}_4)_2$ . During the iFADO cruise, the same overall results were observed for both the SHI2600 and PE850 spectrophotometers:  $R$  differences between reagents ( $\text{Pb}(\text{ClO}_4)_2 - \text{PbCl}_2$ ) were  $0.0050 \pm 0.0015$  and  $0.0061 \pm 0.0006$ , respectively (data not shown). In this regard, the possibility that perchlorate ( $\text{ClO}_4^-$ ) could be absorbing light at the target wavelengths was examined using a solution of  $\text{ClO}_4^-$  (>98% purity) in different seawater conditions in terms of salinity and  $[\text{CO}_3^{2-}]_{\text{calc}}$  showing that

measured absorbances were not different from zero at the target wavelengths (results not shown).

During the iFADO cruise, further comparison experiments of reagents and spectrophotometers were performed on quadruplicate samples through scan measurements (Appendix F). The observed results show that  $_{234}A$  and  $_{250}A$  are always higher when measured using  $\text{Pb}(\text{ClO}_4)_2$  compared to  $\text{PbCl}_2$  (Figure S6), which is expected considering that the final Pb(II) concentration in the cuvette is higher when using  $\text{Pb}(\text{ClO}_4)_2$  (Table S1).  $_{234}A$  and  $_{250}A$  measurements obtained with different spectrophotometers are broadly coincident for data measured with  $\text{PbCl}_2$  (Figure S6A,B), which is also the case for  $_{250}A$  data measured with  $\text{Pb}(\text{ClO}_4)_2$  (Figure S6D). While a good agreement was observed between the SHI2600 and PE850 spectrophotometers for the measurements of  $_{234}A$  and  $_{250}A$  using  $\text{PbCl}_2$  (Figure S6A,B), only measurements of  $_{250}A$  agreed between the two instruments when  $\text{Pb}(\text{ClO}_4)_2$  was used (Figure S6D). In fact,  $_{234}A$  values measured with  $\text{Pb}(\text{ClO}_4)_2$  clearly deviate from the 1:1 line, with SHI2600 yielding higher values than PE850 (Figure S6C). These results are well depicted in Figure S7A, showing the overlapping of  $_{250}A$  versus  $_{234}A$  measured with  $\text{PbCl}_2$  for both spectrophotometers. However, Figure S7B also shows that  $\text{Pb}(\text{ClO}_4)_2$  data split into two groups depending on the spectrophotometer used. Consequently,  $R$  values from  $\text{PbCl}_2$  are comparable between SHI2600 and PE850, but PE850 yields higher  $R$  values when using  $\text{Pb}(\text{ClO}_4)_2$  (Figure S7C).

The observed results are surprising as larger differences in the  $_{250}A$  value were expected because it is located in a slope area. No sampling, preservation, or manipulation differences between replicates can be ascribed to the observed results. Considering the similar technical specifications between SHI2600 and PE850 in terms of wavelength and photometric accuracy (Table S3), and the fact that mean  $_{234}A$  and  $_{250}A$  integrate absorbance data around  $\pm 2$  nm of the target wavelengths (Appendix F), the only difference between them is the stray light specification (Appendix C). However, this would lead to  $_{234}A$  PE850 >  $_{234}A$  SHI2600, which is opposite to the observed results.

In conclusion, the change in Pb(II) reagent seems to affect the determination of  $[\text{CO}_3^{2-}]_{\text{spec}}$ . Using  $\text{Pb}(\text{ClO}_4)_2$  improves data dispersion (Figure 2) regarding  $\text{PbCl}_2$ , but  $\text{Pb}(\text{ClO}_4)_2$  also appears to be more sensitive to inaccuracies in the absorbance signal related to the technical specifications of the equipment.

**4.3. In Situ Temperature Correction.** The approaches by BY08, EAS13, PAT15, and SHA17 need temperature control at  $25 \text{ }^\circ\text{C} \pm 0.05 \text{ }^\circ\text{C}$  (Table S1), while SHA19 introduced temperature-dependent terms in the absorptivity coefficients and in the formation constant (Table S2) that allow determinations over a range of temperatures ( $3 \text{ }^\circ\text{C} < t \pm 0.05 \text{ }^\circ\text{C} < 40 \text{ }^\circ\text{C}$ ; Table S1). Recall that Soli et al.<sup>31</sup> reported that the formation constant (eq S3) is almost constant for the range 15–35  $^\circ\text{C}$ . This is reflected in Table S2 where the temperature dependence of the formation constant is minor, while the absorptivity terms have stronger temperature dependence. SHA19 reported an error of about 3% in measured  $[\text{CO}_3^{2-}]_{\text{specSHA19}}$  for 1  $^\circ\text{C}$  bias in temperature. Using the SHA19 approach and the temperature recordings for each sample, the observed bias in  $[\text{CO}_3^{2-}]_{\text{spec}}$  for samples that lacked temperature control at 25  $^\circ\text{C}$  (Figure 4E, F) is in agreement with the bias reported by SHA19. Hence,  $[\text{CO}_3^{2-}]_{\text{spec}}$  is underestimated in samples with a temperature higher than 25  $^\circ\text{C}$  that are incorrectly reported at 25  $^\circ\text{C}$ , underestimating  $[\text{CO}_3^{2-}]_{\text{spec}}$  by about  $5 \mu\text{mol}\cdot\text{kg}^{-1}$  ( $\approx 3\%$ ) for 1  $^\circ\text{C}$  positive bias in



temperature. All the approaches recommend temperature control within  $\pm 0.05$  °C (Table S1), and the results of this study suggest that temperature control is needed at least within  $\pm 1$  °C to reduce uncertainty within the  $\pm 4$  % limit.

## 5. CONCLUSIONS

The assessment of the internal consistency between  $[\text{CO}_3^{2-}]_{\text{spec}}$  from the five different approaches of the methodology and  $[\text{CO}_3^{2-}]_{\text{calc}}$  according to data in this study allowed a detailed comparison of the differential factors among the evolving approaches studied, regarding the respective sets of calibration functions to infer  $[\text{CO}_3^{2-}]_{\text{spec}}$  (Table S2) as well as an examination of other methodological updates proposed through time (Table S1). Overall results suggest that further documentation is needed until  $[\text{CO}_3^{2-}]_{\text{spec}}$  can be implemented as the fifth measurable variable of the seawater  $\text{CO}_2$  system. A summary of areas where improvement is needed to enhance the long-term reproducibility of  $[\text{CO}_3^{2-}]_{\text{spec}}$  to warrant the broader implementation of  $[\text{CO}_3^{2-}]_{\text{spec}}$  measurements are detailed in the following:

- (i) Current robustness of  $[\text{CO}_3^{2-}]_{\text{spec}}$  for OA monitoring studies.  $[\text{CO}_3^{2-}]_{\text{spec}}$  observations reported in this study suggest that approaches of the methodology assessed (BY08, EAS13, PAT15, SHA17, and SHA19; Table S1) are not yet ready for applications that require climate-quality measurements because they do not meet the GOA-ON objective of  $\pm 1$  % standard uncertainty for the whole studied range of  $[\text{CO}_3^{2-}]_{\text{calc}}$ . Moreover, none of the five approaches assessed is clearly the best option for being globally implemented. But all the approaches except PAT15 fulfill the weather-quality standard of  $\pm 10$  %. Those approaches proven to meet the weather-quality objective could be used and further tested in studies facing large temporal or spatial variability in  $[\text{CO}_3^{2-}]$  or in other compatible applications like OA experimentation in aquaria, shellfish aquaculture, or coastal conservation.
- (ii)  $[\text{CO}_3^{2-}]_{\text{spec}}$  as the fifth  $\text{CO}_2$  measurable variable and internal consistency analysis of  $\text{CO}_2$  overdetermined systems. Few  $[\text{CO}_3^{2-}]_{\text{spec}}$  observations reported in this study meet the expected  $\pm 2$  % standard uncertainty attained in reference bibliography (Table S1). Furthermore, the relative  $\Delta[\text{CO}_3^{2-}]$  distribution between approaches remains the same for the entire salinity and  $[\text{CO}_3^{2-}]_{\text{calc}}$  ranges studied, where  $[\text{CO}_3^{2-}]_{\text{specBY08}} \approx [\text{CO}_3^{2-}]_{\text{specEAS13}} < [\text{CO}_3^{2-}]_{\text{specSHA17}} \approx [\text{CO}_3^{2-}]_{\text{specSHA19}} < [\text{CO}_3^{2-}]_{\text{specPAT15}}$  but demonstrates an overall lack of consistency between them. This implies that using diverse  $R$  data sets with newer algorithms does not guarantee an improvement in the recalculated data set, which is particularly unfavorable for the maintenance of time-series. Time-series or data sets tracking the  $[\text{CO}_3^{2-}]_{\text{spec}}$  methodological evolution (Table S1) would lack consistency between results obtained with former procedures (BY08 and EAS13) with regard to the most recent approaches from SHA17, SHA19, and PAT15. According to these findings, it might not be recommendable to include  $[\text{CO}_3^{2-}]_{\text{spec}}$  as the fifth  $\text{CO}_2$  measurable variable until the methodology is extensively reviewed and implemented by more research groups. There are few references from independent groups reporting the use of the  $[\text{CO}_3^{2-}]_{\text{spec}}$  methodology,<sup>44</sup> which is a clear disadvantage for its widespread implementation as a

well-tested method. This point was considered in the GLODAPv2.2020 update where no  $[\text{CO}_3^{2-}]$  data were included.<sup>36</sup> The inclusion of  $[\text{CO}_3^{2-}]_{\text{spec}}$  as the fifth measurable variable with any of the approaches for internal consistency studies would likely add noise in the already complicated seawater  $\text{CO}_2$  system modeling and characterization, where known inconsistencies are currently under debate.<sup>38,51</sup> Additionally, caution is needed when pairing  $[\text{CO}_3^{2-}]_{\text{spec}}$  with another seawater  $\text{CO}_2$  variable to estimate the whole seawater  $\text{CO}_2$  system.<sup>25</sup> According to the observed results, a standard uncertainty larger than 2 % should be assigned to  $[\text{CO}_3^{2-}]_{\text{spec}}$  to evaluate propagated uncertainties in derived  $\text{CO}_2$  variables.

- (iii) SOP for  $[\text{CO}_3^{2-}]_{\text{spec}}$  measurements and factors to be further specified. This study highlights several inconsistencies in the  $[\text{CO}_3^{2-}]_{\text{spec}}$  methodology evolution related to the Pb(II) reagent, the equipment specifications, and controversial perturbation and wavelength offset corrections, which points to the need to provide a well-described SOP for end-users, as available for the other four seawater  $\text{CO}_2$  system variables<sup>17</sup> that allows the successful performance of the method in diverse seawater conditions. A summary of likely significant factors that should be revisited and made clearer to users follows.

**5.1. Spectrophotometer.** The technical specifications regarding photometric and wavelength accuracies and the stray light seem crucial for  $[\text{CO}_3^{2-}]_{\text{spec}}$  determination. The observed  $\Delta[\text{CO}_3^{2-}]$  values reflect the dependence between the degree of data dispersion and the photometric accuracy of the spectrophotometer. The stray light seems to cause significant differences in  $_{234A}$  between spectrophotometers when  $\text{Pb}(\text{ClO}_4)_2$  is used, but the reason is unknown. Additionally, the use of this reagent demands the assessment of an offset correction ( $\Delta\lambda_{241.1}$ ; Table S1) related to the wavelength accuracy of the equipment to correct systematic biases in the data. However,  $\Delta\lambda_{241.1}$  assessment and implementation should be described more clearly since it seems controversial, going beyond the limits of uncertainty of both the wavelength accuracy specifications of the spectrophotometers and the holmium oxide certified standard accuracy.

**5.2. Pb(II) Reagent.**  $R$  values obtained with  $\text{Pb}(\text{ClO}_4)_2$  are about 0.004–0.006 units higher than  $R$  measured with  $\text{PbCl}_2$ . Such difference seems insignificant when introduced in the formulations of the different approaches for calculating  $[\text{CO}_3^{2-}]_{\text{spec}}$ . In this regard,  $\Delta[\text{CO}_3^{2-}]$  showed less dispersion for data measured with  $\text{Pb}(\text{ClO}_4)_2$ , which would support the reagent change. Nevertheless,  $\text{Pb}(\text{ClO}_4)_2$  might cause the  $_{234A}$  characterization to become more sensitive to the spectrophotometer specifications, thus impacting  $R$  measurements to a larger extent than when using  $\text{PbCl}_2$ . Differences in  $R$  values measured with the two Pb(II) reagents should be assessed to ensure the production of consistent data sets between groups and in time.

**5.3. Temperature Sensitivity.** Temperature control is needed within  $\pm 0.05$  °C to obtain  $[\text{CO}_3^{2-}]_{\text{spec}}$  as accurate as possible within the capabilities of the methodology or at least within  $\pm 1$  °C to keep the uncertainty within the  $\pm 4$  % limit attributable to internal consistency.

**5.4. Ranges of Salinity and pH Validity.** The salinity ranges assessed to fit the various sets of calibration functions might impact the accuracy of the resulting  $[\text{CO}_3^{2-}]_{\text{spec}}$  and the

applicability of a given approach. Valid salinity ranges for the BY08 and EAS13 approaches comprise the Atlantic Ocean but not high-salinity waters ( $S > 36.5$ ) where they underestimate  $[\text{CO}_3^{2-}]_{\text{spec}}$ . Overestimation of  $[\text{CO}_3^{2-}]_{\text{spec}}$  is observed, for both the Atlantic Ocean and the Mediterranean Sea with the approaches of PAT15, SHA17, and SHA19. The approaches of BY08 and SHA19 characterized the calibration functions for large salinity ranges:  $20 < S < 36$  and  $20 < S < 40$ , respectively (Table S1). However, these salinity ranges were reached through modification of natural seawater in the laboratory. In BY08 all data was experimental, while in SHA19 they used data from natural samples but merged them with experimental data with broader salinity conditions. The salinity range assessed with natural seawater samples for characterizing the sets of calibration functions is shorter:  $26.6 < S < 36.72$ , among approaches (Table S1). Although the five sets of calibration functions showed the lowest  $[\text{CO}_3^{2-}]_{\text{spec}}$  uncertainties at the lower ranges of  $[\text{CO}_3^{2-}]_{\text{calc}}$  (Figures 3 and S5), suggesting that this would likely apply for seawater at lower salinities than the lowest ranges in this study (i.e.,  $S < 33.7$ ), observational evidence is needed to confirm this. Further  $[\text{CO}_3^{2-}]_{\text{spec}}$  observations are also recommendable for high-salinity waters. Ideally, a reevaluation of the calibration functions should be performed using only data from natural seawater samples.

The existence of five approaches that show inconsistencies among them discourages widespread  $[\text{CO}_3^{2-}]_{\text{spec}}$  determination. The ocean  $\text{CO}_2$  community would benefit from an SOP and the availability of CRMs for  $[\text{CO}_3^{2-}]_{\text{spec}}$  measurement. The SOP should include well-described and validated best practices to be implemented unambiguously by other users interested in setting up  $[\text{CO}_3^{2-}]_{\text{spec}}$  measurements.

## ■ ASSOCIATED CONTENT

### SI Supporting Information

The Supporting Information is available free of charge at <https://pubs.acs.org/doi/10.1021/acs.est.1c06083>.

Appendixes showing (A) Global ocean distribution of carbonate ion content and saturation states. Figure S1. (B) Evolution of the methodology for measuring carbonate ion content, Figures S2 and S3 and Tables S1 and S2. (C) Terminology, Table S3. (D)  $\Delta[\text{CO}_3^{2-}]$  uncertainty assessment: uncertainty in  $[\text{CO}_3^{2-}]_{\text{calc}}$  estimation, Figure S4 and Tables S4 and S5. (E)  $\Delta[\text{CO}_3^{2-}]$  uncertainty assessment:  $[\text{CO}_3^{2-}]_{\text{spec}}$  uncertainty related to the absorbance ratio. Monte Carlo analysis, Figure S5. (F)  $\Delta[\text{CO}_3^{2-}]$  uncertainty assessment:  $[\text{CO}_3^{2-}]_{\text{spec}}$  uncertainty related to the absorbance ratio. Absorbance measurements with both Pb(II) reagents and different spectrophotometers, Figures S6 and S7 (PDF)

## ■ AUTHOR INFORMATION

### Corresponding Author

Elisa F. Guallart — Centro Oceanográfico de A Coruña (COAC-IEO), CSIC, DC 15001 A Coruña, Spain; Institut de Ciències del Mar (ICM), CSIC, DC 08003 Barcelona, Spain; [orcid.org/0000-0003-2965-6671](https://orcid.org/0000-0003-2965-6671); Phone: (+34) 932309500; Email: [efguallart@icm.csic.es](mailto:efguallart@icm.csic.es); Fax: (+34) 932309555

## Authors

Noelia M. Fajar — Centro Oceanográfico de A Coruña (COAC-IEO), CSIC, DC 15001 A Coruña, Spain; Instituto de Investigaciones Mariñas (IIM), CSIC, DC 36208 Vigo, Spain  
Maribel I. García-Ibáñez — School of Environmental Sciences, University of East Anglia (UEA), Norwich NR47TJ, United Kingdom; Institut de Ciències del Mar (ICM), CSIC, DC 08003 Barcelona, Spain; [orcid.org/0000-0001-5218-0064](https://orcid.org/0000-0001-5218-0064)  
Mónica Castaño-Carrera — Centro Oceanográfico de A Coruña (COAC-IEO), CSIC, DC 15001 A Coruña, Spain  
Rocio Santiago-Doménech — Centro Oceanográfico de Baleares (COB-IEO), CSIC, DC 07015 Palma de Mallorca, Balearic Islands, Spain  
Abd El Rahman Hassoun — GEOMAR Helmholtz Centre for Ocean Research Kiel, D-24105 Kiel, Germany; National Center for Marine Sciences, National Council for Scientific Research in Lebanon (CNRS-L), Beirut, Lebanon; [orcid.org/0000-0003-1940-215X](https://orcid.org/0000-0003-1940-215X)  
Fiz F. Pérez — Instituto de Investigaciones Mariñas (IIM), CSIC, DC 36208 Vigo, Spain  
Regina A. Easley — Chemical Sciences Division, National Institute of Standards and Technology (NIST), DC 20899 Gaithersburg, Maryland, United States  
Marta Álvarez — Centro Oceanográfico de A Coruña (COAC-IEO), CSIC, DC 15001 A Coruña, Spain; [orcid.org/0000-0002-5075-9344](https://orcid.org/0000-0002-5075-9344)

Complete contact information is available at:

<https://pubs.acs.org/doi/10.1021/acs.est.1c06083>

## Author Contributions

□E.F.G. and M.A. contributed equally to this work. All authors contributed to the interpretation of the data and the discussion of the results presented in the manuscript. All authors have given approval to the final version of the manuscript.

## Funding

E.F.G. was supported by a Personal Técnico de Apoyo contract (PTA2016-12441-I) and N.M.F. was supported by a Juan de la Cierva postdoctoral contract (FJCI2015-24394), both from the Spanish Ministry of Science, Innovation and Universities and GAIN Grupo de Referencia Competitiva IN607A 2018/2 from Xunta de Galicia. M.I.G.-I. was supported by NOAA's Ocean Acidification Program (OAP) via Award No. NA17OAR0170332, and by NERC's CUSTARD (Carbon Uptake and Seasonal Traits of Antarctic Remineralisation Depths) project NE/P021263/1. A.E.R.H. was supported via the 2018 NF-POGO Shipboard Fellowship. F.F.P. was supported by the BOCATS2 (PID2019-104279GB-C21/AEI/10.13039/501100011033) project funded by MCIN/AEI/10.13039/501100011033 and contributing to WATER:iOS CSIC PTI. M.A. was supported by IEO RADIALES, RADPROF, and MEDSHIP18 programs. The MEDWAVES cruise was funded under the ATLAS project (Grant Agreement No. 678760). The RADPROF (2020) cruise was funded under the INTERREG Atlantic Area iFADO project. Useful and related discussions were held at the Ocean Carbonate System Intercomparison Forum working group funded by the Ocean Carbon Biogeochemistry program.

## Notes

The authors declare no competing financial interest.

## ACKNOWLEDGMENTS

This work was possible thanks to the commitment of agencies, principal investigators, scientists, technicians, and crew members acquiring high-quality hydrographic and biogeochemical data on transoceanic cruises and making them publicly available. The authors would like to thank Dr. Michael R. Winchester, Dr. Paul C. De Rose, and Dr. Jason F. Waters (NIST Materials Measurement Laboratory) for their helpful reviews. Certain commercial equipment, instruments, or materials are identified in this paper to specify the experimental procedure adequately. Such identification is not intended to imply recommendation or endorsement by NIST, nor is it intended to imply that the materials or equipment identified are necessarily the best available for the purpose. We are grateful for the comments of Dr. Andrew Dickson, Dr. Simone Alin, and a third anonymous reviewer.

## ABBREVIATIONS

BK800	Beckman DU800 spectrophotometer
BY08	approach for measuring $[\text{CO}_3^{2-}]_{\text{spec}}$ described by Byrne and Yao <sup>24</sup>
$\text{CO}_2$	carbon dioxide
$[\text{CO}_3^{2-}]_{\text{calc}}$	calculated carbonate ion content from pH-TA or DIC-TA pairs
$[\text{CO}_3^{2-}]_{\text{spec}}$	spectrophotometric carbonate ion content
DIC	dissolved inorganic carbon
EAS13	approach for measuring $[\text{CO}_3^{2-}]_{\text{spec}}$ described by Easley et al. <sup>28</sup>
GOA-ON	Global Ocean Acidification Observing Network
OA	ocean acidification
PAT15	approach for measuring $[\text{CO}_3^{2-}]_{\text{spec}}$ described by Patsavas et al. <sup>29</sup>
PE850	PerkinElmer Lambda 850 spectrophotometer
R	absorbance ratio
SHA17	approach for measuring $[\text{CO}_3^{2-}]_{\text{spec}}$ described by Sharp et al. <sup>30</sup>
SHA19	approach for measuring $[\text{CO}_3^{2-}]_{\text{spec}}$ described by Sharp and Byrne <sup>25</sup>
SHI2401	Shimadzu UV2401 spectrophotometer
SHI2600	Shimadzu UV2600 spectrophotometer
TA	Total alkalinity

## REFERENCES

- (1) Friedlingstein, P.; Jones, M. W.; O'Sullivan, M.; Andrew, R. M.; Bakker, D. C. E.; Hauck, J.; Le Quéré, C.; Peters, G. P.; Peters, W.; Pongratz, J.; Sitch, S.; Canadell, J. G.; Ciais, P.; Jackson, R. B.; Alin, S. R.; Anthoni, P.; Bates, N. R.; Becker, M.; Bellouin, N.; Bopp, L.; Chau, T. T. T.; Chevallier, F.; Chini, L. P.; Cronin, M.; Currie, K. I.; Decharme, B.; Djeutchouang, L.; Dou, X.; Evans, W.; Feely, R. A.; Feng, L.; Gasser, T.; Gilfillan, D.; Gkritzalis, T.; Grassi, G.; Gregor, L.; Gruber, N.; Gürses, Ö.; Harris, I.; Houghton, R. A.; Hurtt, G. C.; Iida, Y.; Ilyina, T.; Luijkx, I. T.; Jain, A. K.; Jones, S. D.; Kato, E.; Kennedy, D.; Klein Goldewijk, K.; Knauer, J.; Korsbakken, J. I.; Körtzinger, A.; Landschützer, P.; Lauvset, S. K.; Lefèvre, N.; Lienert, S.; Liu, J.; Marland, G.; McGuire, P. C.; Melton, J. R.; Munro, D. R.; Nabel, J. E. M. S.; Nakaoka, S.-I.; Niwa, Y.; Ono, T.; Pierrot, D.; Poulter, B.; Rehder, G.; Resplandy, L.; Robertson, E.; Rödenbeck, C.; Rosan, T. M.; Schwinger, J.; Schwingshackl, C.; Séférian, R.; Sutton, A. J.; Sweeney, C.; Tanhua, T.; Tans, P. P.; Tian, H.; Tilbrook, B.; Tubiello, F.; van der Werf, G.; Vuichard, N.; Wada, C.; Wanninkhof, R.; Watson, A.; Willis, D.; Wiltshire, A. J.; Yuan, W.; Yue, C.; Yue, X.; Zaehle, S.; Zeng, J. Global Carbon Budget 2021. *Earth Syst. Sci. Data Discuss.* **2021**, 2021, 1–191.
- (2) Doney, S. C.; Fabry, V. J.; Feely, R. A.; Kleypas, J. A. Ocean Acidification: The Other  $\text{CO}_2$  Problem. *Annu. Rev. Marine Sci.* **2009**, 1, 169–192.
- (3) Sabine, C. L.; Feely, R. A.; Gruber, N.; Key, R. M.; Lee, K.; Bullister, J. L.; Wanninkhof, R.; Wong, C. S.; Wallace, D. W. R.; Tilbrook, B.; Millero, F. J.; Peng, T.-H.; Kozyr, A.; Ono, T.; Rios, A. F. The Oceanic Sink for Anthropogenic  $\text{CO}_2$ . *Science* **2004**, 305 (5682), 367–371.
- (4) Manabe, S.; Stouffer, R. J. Role of Ocean in Global Warming. *Journal of the Meteorological Society of Japan. Ser. II* **2007**, 85B, 385–403.
- (5) Xie, S.-P. Ocean Warming Pattern Effect On Global And Regional Climate Change. *AGU Advances* **2020**, 1 (1), e2019AV000130.
- (6) Long, S.-M.; Xie, S.-P.; Du, Y.; Liu, Q.; Zheng, X.-T.; Huang, G.; Hu, K.-M.; Ying, J. Effects of Ocean Slow Response under Low Warming Targets. *Journal of Climate* **2020**, 33 (2), 477–496.
- (7) Carstensen, J.; Duarte, C. M. Drivers of pH Variability in Coastal Ecosystems. *Environ. Sci. Technol.* **2019**, 53 (8), 4020–4029.
- (8) Bates, N.; Astor, Y.; Church, M.; Currie, K.; Dore, J.; Gonaalez-Davila, M.; Lorenzoni, L.; Muller-Karger, F.; Olafsson, J.; Santa-Casiano, M. A Time-Series View of Changing Surface Ocean Chemistry Due to Ocean Uptake of Anthropogenic  $\text{CO}_2$  and Ocean Acidification. *Oceanography* **2014**, 27 (1), 126–141.
- (9) Talley, L. D.; Feely, R. A.; Sloyan, B. M.; Wanninkhof, R.; Baringer, M. O.; Bullister, J. L.; Carlson, C. A.; Doney, S. C.; Fine, R. A.; Firing, E.; Gruber, N.; Hansell, D. A.; Ishii, M.; Johnson, G. C.; Katsumata, K.; Key, R. M.; Kramp, M.; Langdon, C.; Macdonald, A. M.; Mathis, J. T.; McDonagh, E. L.; Mecking, S.; Millero, F. J.; Mordy, C. W.; Nakano, T.; Sabine, C. L.; Smethie, W. M.; Swift, J. H.; Tanhua, T.; Thurnherr, A. M.; Warner, M. J.; Zhang, J.-Z. Changes in Ocean Heat, Carbon Content, and Ventilation: A Review of the First Decade of GO-SHIP Global Repeat Hydrography. *Annu. Rev. Mar. Sci.* **2016**, 8 (1), 185–215.
- (10) Hopkins, F. E.; Suntharalingam, P.; Gehlen, M.; Andrews, O.; Archer, S. D.; Bopp, L.; Buitenhuis, E.; Dadou, I.; Duce, R.; Goris, N.; Jickells, T.; Johnson, M.; Keng, F.; Law, C. S.; Lee, K.; Liss, P. S.; Lizotte, M.; Malin, G.; Murrell, J. C.; Naik, H.; Rees, A. P.; Schwinger, J.; Williamson, P. The Impacts of Ocean Acidification on Marine Trace Gases and the Implications for Atmospheric Chemistry and Climate. *Proc. R. Soc. A* **2020**, 476 (2237), 20190769.
- (11) Feely, R. A.; Doney, S. C.; Cooley, S. R. Ocean Acidification. *Oceanography* **2009**, 22 (4), 36–47.
- (12) Andersson, A. J.; Kline, D. I.; Edmunds, P. J.; Archer, S. D.; Bednaršek, N.; Carpenter, R. C.; Chadsey, M.; Goldstein, P.; Grotto, A. G.; Hurst, T. P.; King, A. L.; Kübler, J. E.; Kuffner, I. B.; Mackey, K. R. M.; Menge, B. A.; Paytan, A.; Riebesell, U.; Schnetzer, A.; Warner, M. E.; Zimmerman, R. C. Understanding Ocean Acidification Impacts on Organismal to Ecological Scales. *Oceanography* **2015**, 25 (2), 16–27.
- (13) Doney, S. C.; Busch, D. S.; Cooley, S. R.; Kroeker, K. J. The Impacts of Ocean Acidification on Marine Ecosystems and Reliant Human Communities. *Annu. Rev. Environ. Resour.* **2020**, 45 (1), 83–112.
- (14) Bach, L. T.; Riebesell, U.; Gutowska, M. A.; Federwisch, L.; Schulz, K. G. A Unifying Concept of Coccolithophore Sensitivity to Changing Carbonate Chemistry Embedded in an Ecological Framework. *Progress in Oceanography* **2015**, 135, 125–138.
- (15) Feely, R. A.; Sabine, C. L.; Lee, K.; Berelson, W.; Kleypas, J.; Fabry, V. J.; Millero, F. J. Impact of Anthropogenic  $\text{CO}_2$  on the  $\text{CaCO}_3$  System in the Oceans. *Science* **2004**, 305 (5682), 362–366.
- (16) Zeebe, R. E.; Wolf-Gladrow, D.  *$\text{CO}_2$  in Seawater: Equilibrium, Kinetics, Isotopes*; Elsevier Science, 2001; Vol. 65.
- (17) Dickson, A. G.; Sabine, C. L.; Christian, J. R.; Barger, C. P. *Guide to Best Practices for Ocean  $\text{CO}_2$  Measurements*; PICES special publication; North Pacific Marine Science Organization: Sidney, BC, 2007.
- (18) Riebesell, U.; Fabry, V.; Hansson, L.; Gattuso, J. P. *Guide to Best Practices for Ocean Acidification Research and Data Reporting*; Publications Office of the European Union: LU, 2011.



- (19) Bushinsky, S. M.; Takeshita, Y.; Williams, N. L. Observing Changes in Ocean Carbonate Chemistry: Our Autonomous Future. *Current Climate Change Reports* **2019**, *5* (3), 207–220.
- (20) Claustre, H.; Johnson, K. S.; Takeshita, Y. Observing the Global Ocean with Biogeochemical-Argo. *Annu. Rev. Mar. Sci.* **2020**, *12* (1), 23–48.
- (21) Ma, J.; Shu, H.; Yang, B.; Byrne, R. H.; Yuan, D. Spectrophotometric Determination of pH and Carbonate Ion Concentrations in Seawater: Choices, Constraints and Consequences. *Anal. Chim. Acta* **2019**, *1081*, 18–31.
- (22) Patsavas, M. C.; Byrne, R. H.; Wanninkhof, R.; Feely, R. A.; Cai, W.-J. Internal Consistency of Marine Carbonate System Measurements and Assessments of Aragonite Saturation State: Insights from Two U.S. Coastal Cruises. *Marine Chemistry* **2015**, *176*, 9–20.
- (23) McLaughlin, K.; Weisberg, S.; Dickson, A.; Hofmann, G.; Newton, J.; Aseltine-Neilson, D.; Barton, A.; Cudd, S.; Feely, R.; Jefferds, I.; Jewett, E.; King, T.; Langdon, C.; McAfee, S.; Pleschner-Steele, D.; Steele, B. Core Principles of the California Current Acidification Network: Linking Chemistry, Physics, and Ecological Effects. *oceanog* **2015**, *25* (2), 160–169.
- (24) Byrne, R. H.; Yao, W. Procedures for Measurement of Carbonate Ion Concentrations in Seawater by Direct Spectrophotometric Observations of Pb(II) Complexation. *Marine Chemistry* **2008**, *112* (1), 128–135.
- (25) Sharp, J. D.; Byrne, R. H. Carbonate Ion Concentrations in Seawater: Spectrophotometric Determination at Ambient Temperatures and Evaluation of Propagated Calculation Uncertainties. *Marine Chemistry* **2019**, *209*, 70–80.
- (26) Shangguan, Q.; Shu, H.; Li, P.; Lin, K.; Byrne, R. H.; Li, Q.; Yuan, D.; Ma, J. Automated Spectrophotometric Determination of Carbonate Ion Concentration in Seawater Using a Portable Syringe Pump Based Analyzer. *Marine Chemistry* **2019**, *209*, 120–127.
- (27) Byrne, R. H. Inorganic Lead Complexation in Natural Seawater Determined by UV Spectroscopy. *Nature* **1981**, *290* (5806), 487–489.
- (28) Easley, R. A.; Patsavas, M. C.; Byrne, R. H.; Liu, X.; Feely, R. A.; Mathis, J. T. Spectrophotometric Measurement of Calcium Carbonate Saturation States in Seawater. *Environ. Sci. Technol.* **2013**, *47* (3), 1468–1477.
- (29) Patsavas, M. C.; Byrne, R. H.; Yang, B.; Easley, R. A.; Wanninkhof, R.; Liu, X. Procedures for Direct Spectrophotometric Determination of Carbonate Ion Concentrations: Measurements in US Gulf of Mexico and East Coast Waters. *Marine Chemistry* **2015**, *168*, 80–85.
- (30) Sharp, J. D.; Byrne, R. H.; Liu, X.; Feely, R. A.; Cuyler, E. E.; Wanninkhof, R.; Alin, S. R. Spectrophotometric Determination of Carbonate Ion Concentrations: Elimination of Instrument-Dependent Offsets and Calculation of In Situ Saturation States. *Environ. Sci. Technol.* **2017**, *51* (16), 9127–9136.
- (31) Soli, A. L.; Stewart, Z. I.; Byrne, R. H. The Influence of Temperature on  $\text{PbCO}_3^0$  Formation in Seawater. *Marine Chemistry* **2008**, *110* (1), 1–6.
- (32) Luo, Y.; Millero, F. J. Stability Constants for the Formation of Lead Chloride Complexes as a Function of Temperature and Ionic Strength. *Geochim. Cosmochim. Acta* **2007**, *71* (2), 326–334.
- (33) Easley, R. A.; Byrne, R. H. The Ionic Strength Dependence of Lead (II) Carbonate Complexation in Perchlorate Media. *Geochim. Cosmochim. Acta* **2011**, *75* (19), 5638–5647.
- (34) Clayton, T. D.; Byrne, R. H. Spectrophotometric Seawater pH Measurements: Total Hydrogen Ion Concentration Scale Calibration of m-Cresol Purple and at-Sea Results. *Deep Sea Research Part I: Oceanographic Research Papers* **1993**, *40* (10), 2115–2129.
- (35) Alvarez, M.; Pérez, F. F.; Fernández Guallart, E.; Castaño, M.; Fajar, N. M.; García-Ibáñez, M. I.; Santiago-Domenech, R.; El Rahman Hassoun, A. Ten Years of Spanish Ion Carbonate Data in the North Atlantic Ocean and Mediterranean Sea. *Digital CSIC*, 2021. DOI: 10.20350/digitalCSIC/13786.
- (36) Olsen, A.; Lange, N.; Key, R. M.; Tanhua, T.; Bittig, H. C.; Kozyr, A.; Alvarez, M.; Azetsu-Scott, K.; Becker, S.; Brown, P. J.; Carter, B. R.; Cotrim da Cunha, L.; Feely, R. A.; van Heuven, S.; Hoppema, M.; Ishii, M.; Jeansson, E.; Jutterström, S.; Landa, C. S.; Lauvset, S. K.; Michaelis, P.; Murata, A.; Pérez, F. F.; Pfeil, B.; Schirnick, C.; Steinfeldt, R.; Suzuki, T.; Tilbrook, B.; Velo, A.; Wanninkhof, R.; Woosley, R. J. An Updated Version of the Global Interior Ocean Biogeochemical Data Product, GLODAPv2.2020. *Earth System Science Data* **2020**, *12* (4), 3653–3678.
- (37) Orr, J. C.; Epitalon, J.-M.; Dickson, A. G.; Gattuso, J.-P. Routine Uncertainty Propagation for the Marine Carbon Dioxide System. *Marine Chemistry* **2018**, *207*, 84–107.
- (38) Álvarez, M.; Fajar, N. M.; Carter, B. R.; Guallart, E. F.; Pérez, F. F.; Woosley, R. J.; Murata, A. Global Ocean Spectrophotometric pH Assessment: Consistent Inconsistencies. *Environ. Sci. Technol.* **2020**, *54* (18), 10977–10988.
- (39) Pérez, F. F.; Rios, A. F.; Rellán, T.; Alvarez, M. Improvements in a Fast Potentiometric Seawater Alkalinity Determination. *Ciencias Marinas* **2000**, *26* (3), 463–478.
- (40) Pérez, F. F.; Fraga, F. A Precise and Rapid Analytical Procedure for Alkalinity Determination. *Marine Chemistry* **1987**, *21* (2), 169–182.
- (41) Mintrop, L.; Pérez, F. F.; González Dávila, M.; Santana-Casiano, J. M.; Körtzinger, A. Alkalinity Determination by Potentiometry: Intercalibration Using Three Different Methods. *Ciencias Marinas* **2000**, *26* (3), 463–478. DOI: 10.7773/cm.v26i1.573
- (42) Johnson, K. M.; Dickson, A. G.; Eiseid, G.; Goyet, C.; Guenther, P.; Key, R. M.; Millero, F. J.; Purkerson, D.; Sabine, C. L.; Schott, R. G.; et al. Coulometric Total Carbon Dioxide Analysis for Marine Studies: Assessment of the Quality of Total Inorganic Carbon Measurements Made during the US Indian Ocean CO<sub>2</sub> Survey 1994–1996. *Marine Chemistry* **1998**, *63* (1–2), 21–37.
- (43) Dickson, A. G.; Afghan, J. D.; Anderson, G. C. Reference Materials for Oceanic CO<sub>2</sub> Analysis: A Method for the Certification of Total Alkalinity. *Marine Chemistry* **2003**, *80* (2), 185–197.
- (44) Fajar, N. M.; García-Ibáñez, M. I.; SanLeón-Bartolomé, H.; Álvarez, M.; Pérez, F. F. Spectrophotometric Measurements of the Carbonate Ion Concentration: Aragonite Saturation States in the Mediterranean Sea and Atlantic Ocean. *Environ. Sci. Technol.* **2015**, *49* (19), 11679–11687.
- (45) Van Heuven, S.; Pierrot, D.; Rae, J. W. B.; Lewis, E.; Wallace, D. W. R. *MATLAB Program Developed for CO<sub>2</sub> System Calculations*; ORNL/CDIAC-105b, 2011; p 530.
- (46) Mehrbach, C.; Culbertson, C. H.; Hawley, J. E.; Pytkowicz, R. M. Measurement of the Apparent Dissociation Constants of Carbonic Acid in Seawater at Atmospheric Pressure. *Limnology and Oceanography* **1973**, *18* (6), 897–907.
- (47) Lueker, T. J.; Dickson, A. G.; Keeling, C. D. Ocean pCO<sub>2</sub> Calculated from Dissolved Inorganic Carbon, Alkalinity, and Equations for K<sub>1</sub> and K<sub>2</sub>: Validation Based on Laboratory Measurements of CO<sub>2</sub> in Gas and Seawater at Equilibrium. *Marine Chemistry* **2000**, *70* (1), 105–119.
- (48) Dickson, A. G. Standard Potential of the Reaction:  $\text{AgCl(s)} + 12\text{H}_2\text{(g)} = \text{Ag(s)} + \text{HCl(aq)}$ , and the Standard Acidity Constant of the Ion  $\text{HSO}_4^-$  in Synthetic Sea Water from 273.15 to 318.15 K. *J. Chem. Thermodyn.* **1990**, *22* (2), 113–127.
- (49) Lee, K.; Kim, T.-W.; Byrne, R. H.; Millero, F. J.; Feely, R. A.; Liu, Y.-M. The Universal Ratio of Boron to Chlorinity for the North Pacific and North Atlantic Oceans. *Geochim. Cosmochim. Acta* **2010**, *74* (6), 1801–1811.
- (50) Newton, J.; Feely, R.; Jewett, E.; Williamson, P.; Mathis, J. *Global Ocean Acidification Observing Network: Requirements and Governance Plan*, 2nd ed.; GOA-ON, 2015, [http://www.goa-on.org/docs/GOA-ON\\_plan\\_print.pdf](http://www.goa-on.org/docs/GOA-ON_plan_print.pdf); p 61.
- (51) Fong, M. B.; Dickson, A. G. Insights from GO-SHIP Hydrography Data into the Thermodynamic Consistency of CO<sub>2</sub> System Measurements in Seawater. *Marine Chemistry* **2019**, *211*, 52–63.